

INSTALLATION GUIDE

DI 015 EN E

GRAVITRONIQUE

Described in EC-type examination certificate N°: LNE-27785



E	2018/03/27	Printer wiring [MDV594], Opening control flap and product return cpt 6, Installation recommendations of probes, Updating of drawings	DSM	MV
D	2017/09/14	Installation and sealing drawing New FORM DOC – Updating of drawings	DSM	XS
C	2016/11/15	Updating of drawings and electrical wiring	DSM	FB
A	2015/05/04	Creation	DSM	AH
Issue	Date	Nature of modifications	Written by	Approved by

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY

THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION

	INSTALLATION GUIDE DI 015 EN E GRAVITRONIQUE	Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C
	This document is available at www.alma-alma.fr	Page 1 / 47

CONTENTS

1. GENERAL RECOMMENDATIONS	4
1.1. MECHANICAL RECOMMENDATIONS	4
1.2. ELECTRICAL RECOMMENDATIONS	5
1.3. PNEUMATIC RECOMMENDATIONS	7
2. GENERAL PRESENTATION	8
2.1. USE ACCORDING TO MID CERTIFICATE	8
2.2. SPECIAL CONDITIONS FOR INSTALLATION IN ANY CASES	8
3. PART LIST	8
4. INSTALLATION AND SEALING DRAWING OF THE GRAVITRONIQUE	11
5. CALCULATOR-INDICATOR MICROCOMPT+ GRAVITRONIQUE	13
5.1. INSTALLATION RECOMMENDATIONS CALCULATOR-INDICATOR MICROCOMPT+	14
5.2. ELECTRICAL WIRING CALCULATOR-INDICATOR MICROCOMPT+.....	15
Terminal assignment of the interface power supply board	16
Terminal assignment of the extension board 4DG (IS)	18
Terminal assignment of the extension board 'sonde AD' 5wires (IS)	19
Terminal assignment of the relay extension board	20
Control box GRAVITRONIQUE	21
Electrical wiring control box.....	22
Pneumatic wiring control box	24
6. ADRIANE TURBINE METER	25
6.1. TURBINE METER ADRIANE DN100-80 243 TTMA WITH SIGHTGLASS	25
6.2. TURBINE ADRIANE DN80-80 243 110x110.....	26
6.3. INSTALLATION AND SEALING RECOMMENDATIONS ADRIANE TURBINE METER.....	27
7. DIFFERENTIAL PRESSURE TRANSMITTER CP3000 ATEX	28
7.1. INSTALLATION RECOMMENDATIONS CP3000 ATEX.....	29
8. NC/NO SOLENOID VALVES KIT ATEX	30
9. END-OF-METERING PROBE / VACUITY SENSOR – DG3001/75	31
9.1. INSTALLATION RECOMMENDATIONS DG3001/75.....	32
10. PRINTER	33
10.1. INSTALLATION RECOMMENDATIONS PRINTER	34
11. CONVERTER 24VDC/24VDC 2.1A 50W	35
12. VACUUM BREAKER	36
12.1. INSTALLATION RECOMMENDATIONS VACUUM BREAKER.....	37
13. DN80 NON-RETURN VALVE KITS	38
13.1. DN80 NON RETURN VALVE KIT, 0.03 BAR CALIBRATED	38
13.2. DN80 NON RETURN VALVE KIT, 0.3 BAR CALIBRATED (EMPTY HOSE OPTION)	39
13.3. INSTALLATION RECOMMENDATIONS DN80 NON-RETURN VALVE KIT	40
14. PNEUMATIC CONTROL VENT VALVE	41
14.1. INSTALLATION RECOMMENDATIONS PNEUMATIC CONTROL VENT VALVE	42

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY

THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION

	INSTALLATION GUIDE DI 015 ENE GRAVITRONIQUE	Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C
	This document is available at www.alma-alma.fr	

15. TEMPERATURE PROBE PT100 – CT1001	43
15.1. INSTALLATION RECOMMENDATIONS TEMPERATURE PROBE.....	44
16. SIGHTGLASS KIT 110X110 ADRIANE TURBINE METER DN80	45
16.1. INSTALLATION RECOMMENDATIONS SIGHTGLASS KIT DN80.....	46
17. KIT FOR MEASURING SYSTEM IDENTIFICATION PLATE.....	47

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY
--

THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION
--

 ALMA	INSTALLATION GUIDE DI 015 EN E GRAVITRONIQUE	Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C
	This document is available at www.alma-alma.fr	Page 3 / 47

1. GENERAL RECOMMENDATIONS

IN ORDER TO AVOID ALL THE PROBLEMS CONCERNING THE INSTALLATION, THE OPERATION AND THE MAINTENANCE OF THE EQUIPMENTS, BEING ABLE TO CREATE INOPPORTUNE FAILURE, PLEASE RESPECT THE FOLLOWING RECOMMENDATIONS.

BEFORE ANY WORK, MAKE SURE THAT THE EQUIPMENTS ARE NOT POWERED.


1.1. MECANICAL RECOMMENDATIONS

- ⇒ Respect the recommendations of the instruction manual specifying the installation, operation and maintenance conditions of the ATEX equipment (instruction manual supplied with the equipment).
- ⇒ Take care to place the equipment in order to facilitate their installation, operation and maintenance by the technicians (working ergonomics).
- ⇒ Take care to position properly the equipment; the display must be readable without any difficulty.
- ⇒ Apply a tightening torque suitable with size and material of the fixation element except particular specifications mentioned on the presentation drawing or in the installation guides.
- ⇒ Mechanically protect the cables with the corrugated conduit if the cables are not ADR (corrugated conduit adapted to vehicles used for "carriage of dangerous goods of road" - hydrocarbons, LPG ... - and meet the requirements of French standard NF R13-903).
- ⇒ Ensure there are a good mechanical strength and a good sealing between cable glands and cables, and between cable glands and corrugated conduit.
- ⇒ Respect cables and corrugated conduit radii of curvature.
- ⇒ Leave enough flexibility to wires in order to avoid any risk of stripping.
- ⇒ Allow the drainage of the water in the lower loop (siphon) of the corrugated conduit (not water retention inside the corrugated conduit).

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY		
THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION		
 ALMA	INSTALLATION GUIDE DI 015 EN E GRAVITRONIQUE	Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C
	This document is available at www.alma-alma.fr	Page 4 / 47

1.2. ELECTRICAL RECOMMENDATIONS

- ⇒ Respect the recommendations of the instruction manual specifying the installation, operation and maintenance conditions of the ATEX equipment (instruction manual supplied with the equipment).
- ⇒ Connect the supply of the equipment downstream cut-out, on the power supply reserved to the measured distribution.
- ⇒ Put a delayed protection of 5A upstream the 24VDC supply to protect equipment in case of reverse polarity or overcurrent.
- ⇒ Use ADR specific cable, if it is not the case, use at minimum a cable resisting to hydrocarbons. Mechanically protect this cable with a corrugated conduit (corrugated conduit adapted to vehicles used for "carriage of dangerous goods by road" - hydrocarbons, LPG ... - and meet the requirements of French standard NF R13-903).
- ⇒ Take care not to damage the terminals of the different electronic boards while wiring.
 - Screw terminals: do not damage the screw heads of the terminals.
 - Use insulated lugs and insulated wire ferrules adapted to the section of wires.
 - Spring terminals: do not block the springs (if a spring is blocked, the electronic board must be replaced).
 - Use flat screwdriver 0.4x2.5 (see fig.1).
 - Insert the screwdriver slightly tilted, then push it perpendicularly to the terminal.
 - Do not exceed the upright position when the screwdriver is down in order not to block the spring.
 - Insert or remove the wire and remove the screwdriver.



- ⇒ Pass the power supply cores (24VDC truck) through the ferrites by carrying out a loop (ALMA supply).
- ⇒ Do not use wires of section higher than 1.5mm².
- ⇒ Do not insert more than two wires in a terminal, if necessary use an insulated twin wire ferrule (unless otherwise indicated).
- ⇒ Strictly respect the polarities of the input/output when wiring, in accordance with serigraphy on the cards and/or with the installation guide indications.
- ⇒ Whenever possible, perform a wired test, after wiring and before powering.
- ⇒ Whenever possible, respect the locations of the cables specified in the installation guide.
- ⇒ Equipment must be connected to the frame ground (external ground connection).
- ⇒ Whenever possible, use shielded cables with a 360° connection through the metal cable glands (see the documentation delivered with the equipment). Otherwise, connect the shields to devices inside the equipment (ground terminal, earth bar, earth boss...).
- ⇒ Whenever possible, label the cables and cores according to the installation guide to facilitate the later maintenance operations.
- ⇒ Respect a homogeneous wire color code.

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY			
THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION			
 ALMA	INSTALLATION GUIDE DI 015 ENE GRAVITRONIQUE	Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C	
This document is available at www.alma-alma.fr			Page 5 / 47

⇒ Printer TMU295: before positioning the printer on its support, check that configuration switches of the data link protocol, located under the printer, are well positioned: No3 on 'ON' and the 7 others on 'OFF'.

⇒ Current of the electrical devices:

Electrical devices	Supply voltage	Minimum current	Maximum current
MICROCOMPT+	24VDC +/-10%	0.7 A	1.5 A
PRINTER	24VDC +/-10%	0.1 A	5.5 A (switch-on)

⇒ Color code according to DIN 47100.

⇒ Code for designation of colours according to IEC 60757 (except FR codes):

FR				EN	IT	ES	DE
Couleurs	Codes		Standard codes CEI 60757	Colours	Colori	Colores	Farbe
Blanc	Bc		WH	White	Bianco	Blanco	Weiß
Marron	Mr		BN	Brown	Marrone	Marrón	Braun
Vert	Vt		GN	Green	Verde	Verde	Grün
Jaune	Jn		YE	Yellow	Giallo	Amarillo	Gelb
Gris	Gr		GY	Grey	Grigio	Gris	Grau
Rose	Rs		PK	Pink	Rosa	Rosa	Lila
Bleu	Bl		BU	Blue	Blu	Azul	Blau
Rouge	Rg		RD	Red	Rosso	Rojo	Rot
Noir	Nr		BK	Black	Nero	Negro	Schwarz
Violet	Vi		VL	Violet	Viola	Violeta	Violett
Orange	Or		OG	Orange	Arancio	Naranja	Orange
Vert/Jaune	V/J		GNYE	Green/Yellow	Verde/Giallo	Verde/Amarillo	Grün/Gelb

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY

THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION

	INSTALLATION GUIDE DI 015 ENE GRAVITRONIQUE	Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C
	This document is available at www.alma-alma.fr	Page 6 / 47

1.3. PNEUMATIC RECOMMENDATIONS

- ⇒ Air must be filtered – from 40 to 20µm. Specific recommendations may be added in the installation guides or on the presentation drawings.
- ⇒ The air lubrication must be permanent and correct to avoid any damage on the pneumatic components.
- ⇒ The air supply pressure to the inlet of the equipment must be at least 6 bar and max 8 bar. Specific recommendations may be added in the installation guides or on the presentation drawings.
- ⇒ The pneumatic supply pipes (6/4) must be cut straight (no slanting cut) and should not be crushed after cutting to prevent leakage on fittings.
- ⇒ Respect the radii of curvature of the pneumatic pipes indicated by the manufacturer.
- ⇒ Use colored pneumatic pipes to ease maintenance operation.
- ⇒ In no case the exhaust holes of the pneumatic organs should be plugged, obstructed, unless if that is clearly specified in the installation guides or on presentation drawings.
- ⇒ The use of muffler is not allowed under any circumstances (fouling, frost...). Put a pneumatic pipe of sufficient length, pointed downwards, so that its end is placed in a protected area ($L = 100$ mm min.).
- ⇒ Pressure unit conversion:

PRESSURE UNIT CONVERSION				
Unités	Bar	PSI	Pascal	kg/cm ²
1 Bar =	1	14,5	100 000 (1x10 ⁵)	1,0197
1 PSI =	0,069	1	6894,5	0,07031
1 Pascal =	1x10 ⁻⁵	14,5x10 ⁻⁵	1	1,0197x10 ⁻⁵
1 kg/cm ² =	0,98	14,22	98066,5	1

PSI = Pound per Square Inch (livre par pouce carré)

1 bar = 100 kPa = 0.1 MPa (1 MPa = 10 bar)

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY		
THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION		
 ALMA	INSTALLATION GUIDE DI 015 ENE GRAVITRONIQUE	Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C
This document is available at www.alma-alma.fr		Page 7 / 47

2. GENERAL PRESENTATION

2.1. USE ACCORDING TO MID CERTIFICATE

The GRAVITRONIQUE measuring system is covered by the EC type examination certificate N° LNE-27785. Refer to this certificate for any precision about its installation.

For the sealing plan, see Annex to EC type examination certificate N° LNE-27785.

2.2. SPECIAL CONDITIONS FOR INSTALLATION IN ANY CASES

- ⇒ Connection pipework between the compartments and the manifold, as between the manifold and the selection valves must have a minimum gradient of 3%.
 - ⇒ Pumped mode: Connection pipework between the selection valve for pumped mode and the pump entry should not include reverse slopes.
- If the measuring system is fitted with several delivery points, it needs to be equipped with a device allowing a liquid delivery by only one point at once.
- ⇒ Gravity mode: If appropriate, the connection pipework between the selection valve for gravity mode and decanting valve must have a minimum gradient of 3%. The vehicle on which the measuring system is installed should have a device to check its horizontality.

3. PART LIST

EQUIPMENTS INCLUDED IN THE MEASURING SYSTEM DELIVERED BY ALMA				
Item	Equipment	Designation	Qty	Option*
1		CALCULATOR INDICATOR MICROCOMPT+ GRAVITRONIQUE (Provided with a magnetic or RFID supervisor key)	1	
2		CONTROL BOX GRAVITRONIQUE	1	
3		ADRIANE TURBINE METER DN100-80 243 TTMA with sightglass (Depending on configuration)	1	
		ADRIANE TURBINE METER DN80-80 243 110x110 (Depending on configuration)		

Non-contractual pictures

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY		
THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION		
	INSTALLATION GUIDE DI 015 ENE GRAVITRONIQUE	Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C
	This document is available at www.alma-alma.fr	Page 8 / 47

EQUIPMENTS INCLUDED IN THE MEASURING SYSTEM DELIVERED BY ALMA				
Item	Equipment	Designation	Qty	Option*
4		DIFFERENTIAL PRESSURE TRANSMITTER – CP3000 ATEX	1	
5		NC/NO ATEX SOLENOID VALVES KIT	1	
6		END-OF-METERING PROBE – DG3001/75 (Supplied if not mounted on the manifold)	1	
		VACUITY SENSOR – DG3001/75 (Supplied if not mounted on the manifold)	1	
7		PRINTER TMU-295 (Printer – power supply cable – serial link cable 10m)	1	
8		CONVERTER 24VDC/24VDC 2.1A 50W (Printer power supply 24VDC)	1	
9		VACUUM BREAKER	1	
10		DN80 NON-RETURN VALVE KIT 0.03 bar	1	
		DN80 NON-RETURN VALVE KIT 0.3 bar (Supplied with an empty hose)	1	•

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY				
THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION				
	INSTALLATION GUIDE DI 015 EN E GRAVITRONIQUE			Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C
This document is available at www.alma-alma.fr			Page 9 / 47	


EQUIPMENTS INCLUDED IN THE MEASURING SYSTEM DELIVERED BY ALMA				
Item	Equipment	Designation	Qty	Option*
11		PNEUMATIC CONTROL VENT VALVE	1	
12		Pt100 TEMPERATURE SENSOR – CT1001-Pe (Supplied with thermowell)	1	●
13		SIGHTGLASS KIT 110x110 ADRIANE TURBINE METER DN80 (Supplied with pre-drilled screws for sealing)	1	
14		KIT FOR MEASURING SYSTEM IDENTIFICATION PLATE (Plate and sealing device)	1	●

Non-contractual pictures

Option*: equipment sold as an option by ALMA, it must be installed on the measuring system if required by the certificate.

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY		
THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION		
	INSTALLATION GUIDE DI 015 ENE GRAVITRONIQUE	Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C
	This document is available at www.alma-alma.fr	

4. INSTALLATION AND SEALING DRAWING OF THE GRAVITRONIQUE

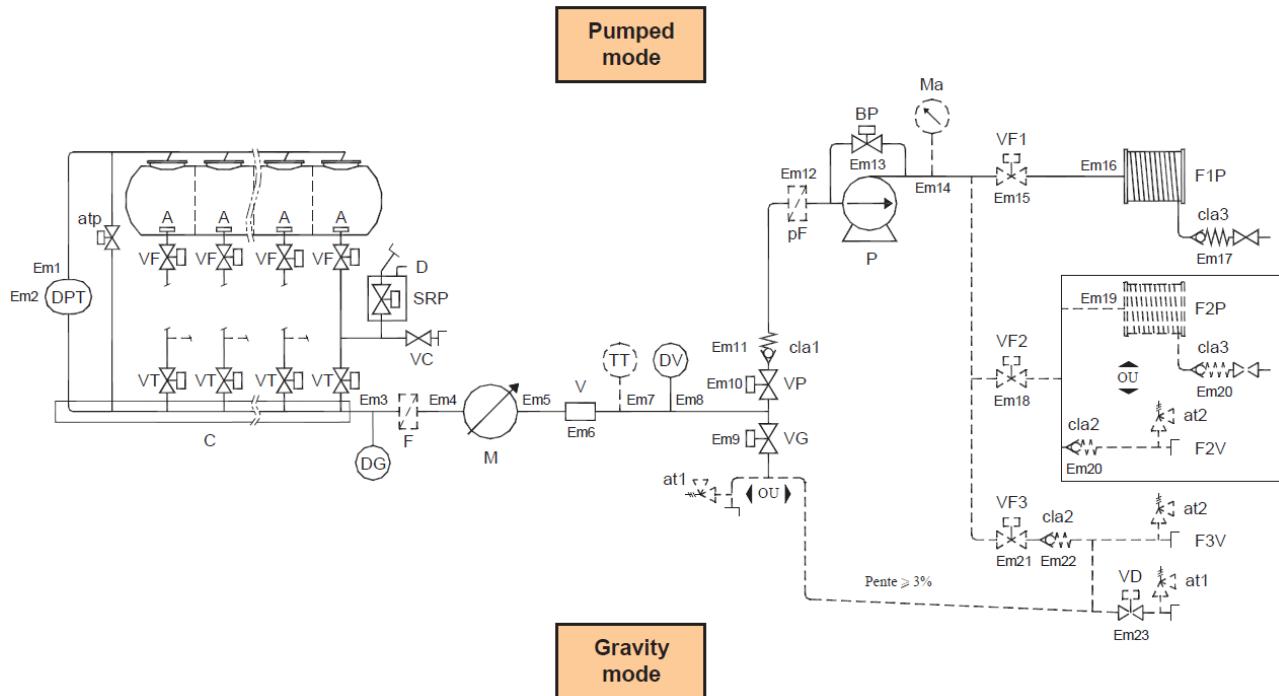

Legend:

- A: Anti-swirl device
- DPT: Pressure sensor
- atp: Guided release to the atmosphere
- VF: Compartment bottom flap
- VT: Selection valve installed on every compartment pipe and allowing transfer to the manifold
- C: Manifold
- D: Pressure relief control (secured)
- SRP: Liquid Backup System on compartments
- VC: Bottom loading valve installed on every compartment pipe (optional)
- DG: gas sensor
- F: Filter (optional if prefilter pF is installed)
- M: Meter
- V: sight glass (can be integrated to the meter)
- TT: Temperature sensor PT100 (optional, and can be integrated to the meter)
- DV: Optical vacuity sensor
- VP: Selection valve pumped mode
- VG: Selection valve gravity mode
- at1, at2: Automatic release to the atmosphere
- cla1: Non-return valve
- pF: Pump prefilter (optional if filter F is installed)
- P: Pump
- BP: Pump by-pass
- Ma: Manometer indicating the forcing back pressure of the pump (optional)
- VF1, VF2, VF3: Device guided by the calculator, allowing, when the measuring system has several pumped delivery paths, to realize deliveries with one or another of these paths (optional). Changing the delivery path is impossible during the measurement.
- F1P, F2P: Full hose(s) on hose reel (F2P optional)
- cla3: Valve calibrated with minimum pressure and preventing the emptying of the full hose.
- cla2: Valve calibrated with minimum pressure at the maximum flowrate of an empty hose (optional)
- F2V, F3V: Connection for empty hose (optional)
- VD: Decanting gravity valve (optional)


ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY		
THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION		
ALMA	INSTALLATION GUIDE DI 015 EN E GRAVITRONIQUE	Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C
This document is available at www.alma-alma.fr		Page 11 / 47

Seals:

- Em1: prevents the removal of pressure sensor DPT.
- Em2: seals the pressure sensor adjustment.
- Em3: prevents the removal of optical sensor DG-3001.
- Em4: seals the inlet pipe of the meter.
- Em5: prevents the removal of the meter.
- Em6: prevents the removal of the sight glass (when not integrated into the meter).
- Em7: prevents the removal of temperature sensor (TT).
- Em8: prevents the removal of vacuity sensor type DG-3001 (DV).
- Em9: prevents the removal of selection valve for gravity mode.
- Em10: prevents the removal of selection valve for pumped mode.
- Em11: prevents the removal of non-return valve for pumped mode.
- Em12: prevents the removal of the prefilter.
- Em13: prevents the removal of the pump and the bypass.
- Em14: prevents the removal of manometer.
- Em15, Em18, Em21: prevent the removal of valves allowing the delivery with empty or full hose(s).
- Em16, Em19: prevents the removal of full hose(s).
- Em17, Em20, Em22: prevents the removal of calibrated non-return valves (transfer point).
- Em23: prevents the removal of decanting valve (VD).

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY		
THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION		
 ALMA	INSTALLATION GUIDE DI 015 EN E GRAVITRONIQUE	Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C
	This document is available at www.alma-alma.fr	Page 12 / 47

5. CALCULATOR-INDICATOR MICROCOMPT+ GRAVITRONIQUE

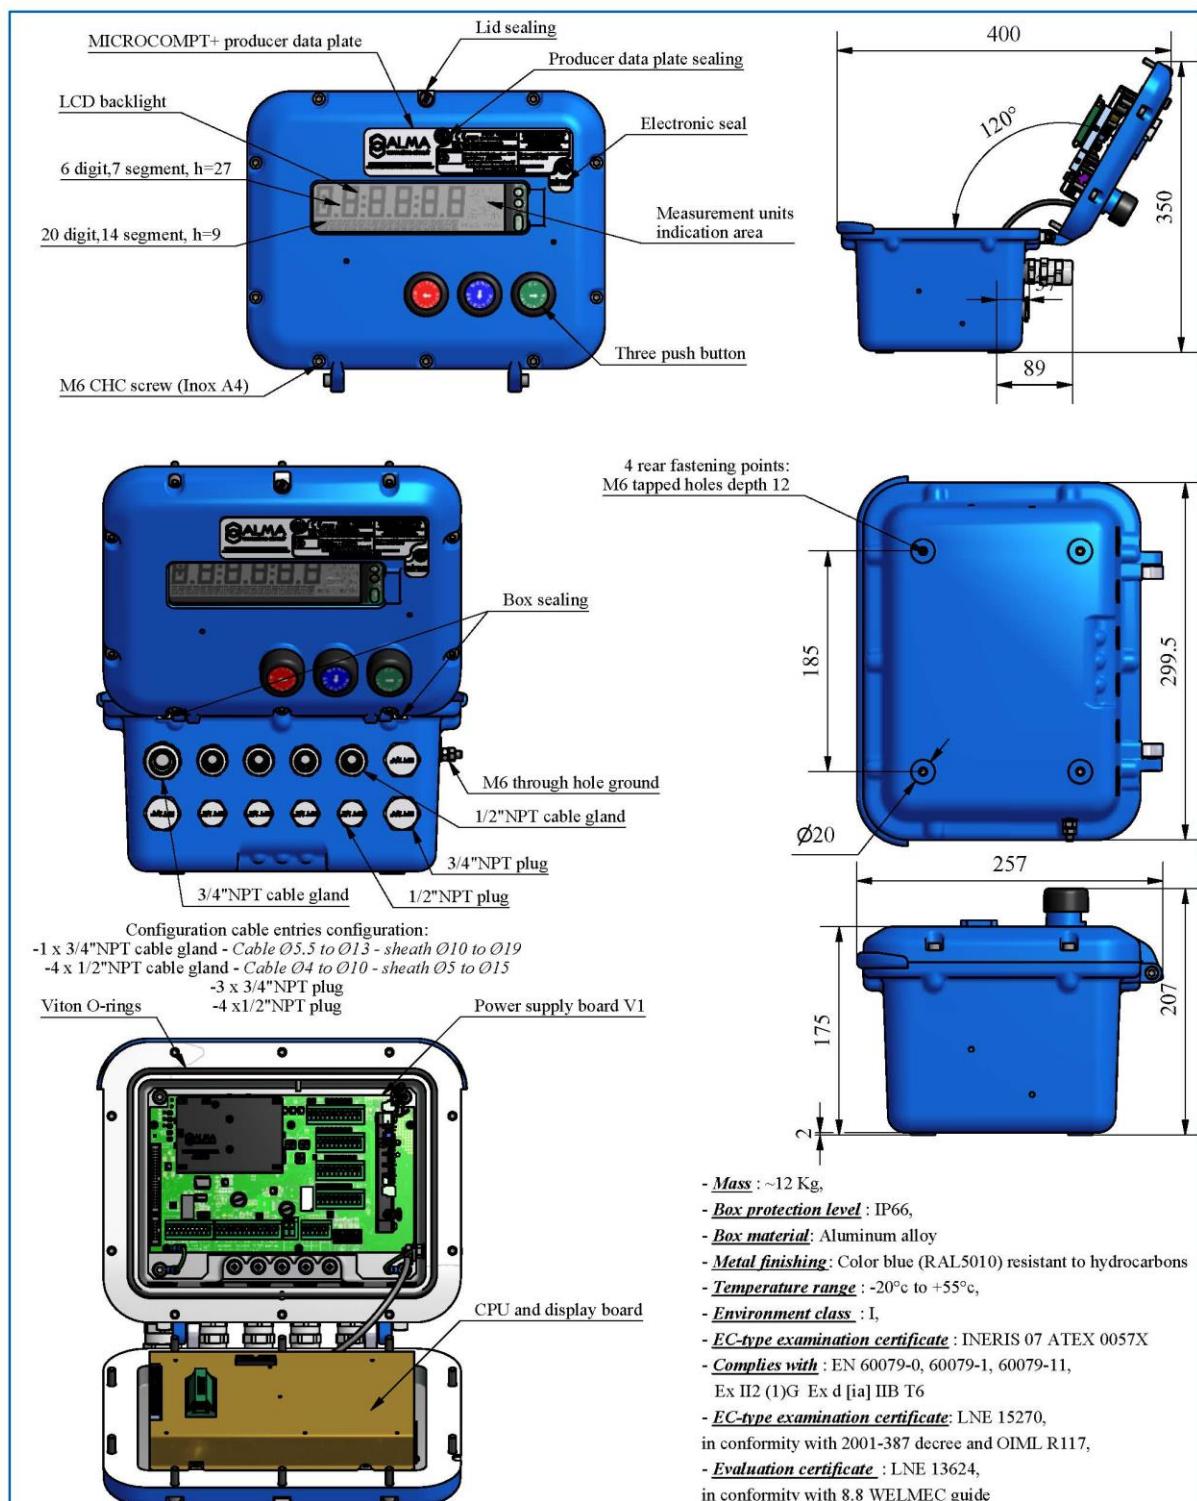

For a safe use of the MICROCOMPT+ electronic device, make sure to comply with the requirements of the instruction manual supplied with the equipment


ALMA www.alma-alma.fr	Service Development 13127 Vitrolles	PRESENTATION DRAWING		DFV094	Description of the amendment N°396 Passage to interface power supply board V1 rev 11 New logo	
		Microcompt+ Gravity metering				
DEV N° : 973	Code : 3695	973	PPV094	I	7/9	Modified on : 17/03/2015 by CC verified by SR
Drawing N° associated with the related CET file	Dev N° Drawing N° Rev Folio	973	PPV094	I	7/9	Created on : 06/12/2010 by CC verified by SR
Metro :	LNE-15270 / LNEI3624					
ATEX:	INERIS 07 ATEX 0057X					

Document available on website [alma-alma.fr](http://www.alma-alma.fr)


ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY						
THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION						
ALMA	INSTALLATION GUIDE DI 015 ENE GRAVITRONIQUE					Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C
	This document is available at www.alma-alma.fr					

5.1. INSTALLATION RECOMMENDATIONS CALCULATOR-INDICATOR MICROCOMPT+


- Fasten the box with 4 M6 screws (holder suitable for vibrations and designed to support the MICROCOMPT). On the box: 4 M6 blind holes tapped length=12 over 185x132).
- Leave an open space around the box in order:
 - o To facilitate maintenance operation.
 - o To prevent any pressing on pushbuttons and on the glass.
- The space between the front face of the box and the cabinet door shall be sufficient.
- Dimensions: A > 100mm and B > 60mm

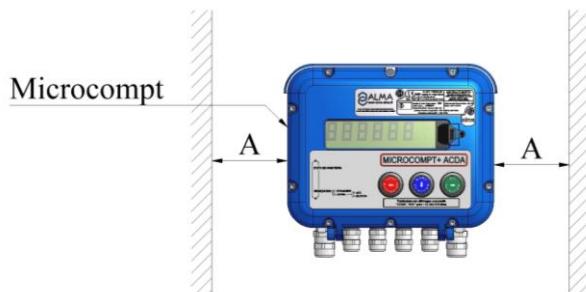

- SOLUTION 1: straight box if it's a breast height.

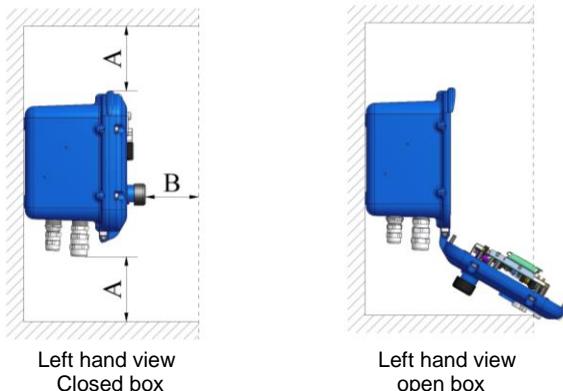

- SOLUTION 2: 20° angle if it's not at breast height.

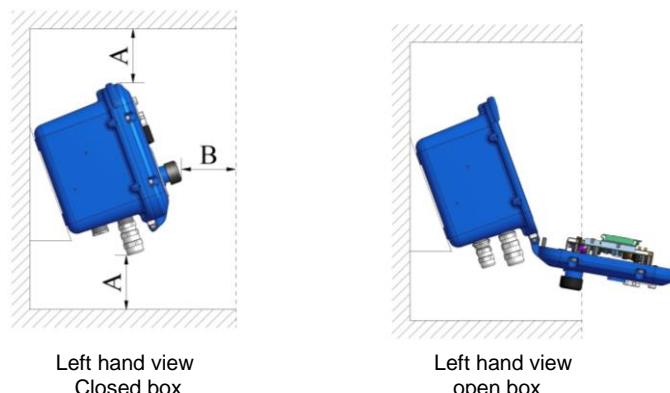


REFER TO THE INSTRUCTION MANUAL

(DELIVERED WITH THE EQUIPMENT OR AVAILABLE ON ALMA WEBSITE)

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY		
THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION		
	INSTALLATION GUIDE DI 015 EN E GRAVITRONIQUE	Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C
This document is available at www.alma-alma.fr		Page 14 / 47

5.2. ELECTRICAL WIRING CALCULATOR-INDICATOR MICROCOMPT+

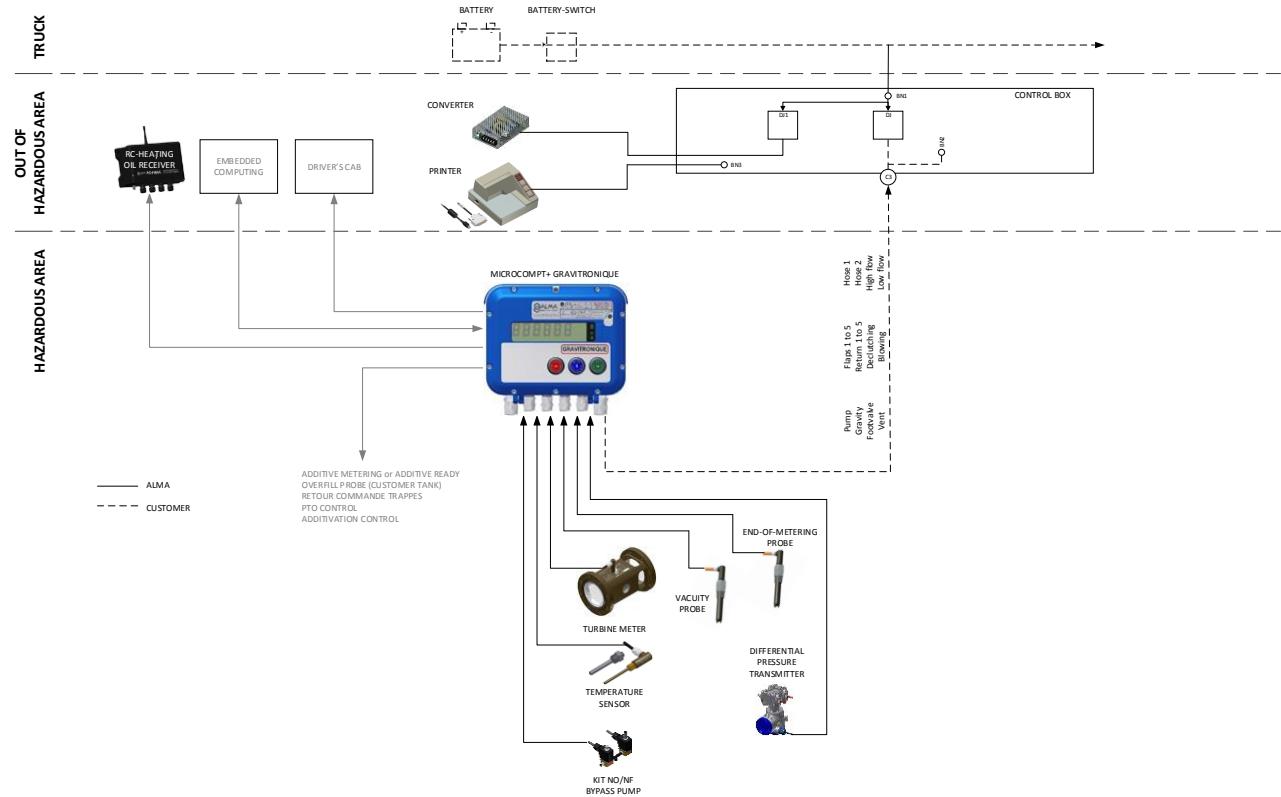

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY

THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION



INSTALLATION GUIDE DI 015 EN E GRAVITRONIQUE

This document is available at www.alma-alma.fr

Units of measure:
 Length: mm
 Angle: degree (° °)
 Temperature: °C

Page 15 / 47

Terminal assignment of the interface power supply board

Any mass braids and shielding must be connected to the MICROCOMPT+ ground bar

TERMINAL ASSIGNMENT OF MICROCOMPT+ BOARDS

INTERFACE POWER SUPPLY BOARD



EQUIPMENTS CONNECTED TO THE MICROCOMPT+

INTERFACE POWER SUPPLY BOARD

Option	Equipment	Cable (for information)				Function	Colour or No.	Terminal	Function		Observation
		No.	CG*	Alma	Type						
	GRAVITRONIQUE CONTROL BOX	C2	1/2"NPT	●	2x1 sh.	Rx Printer		1	Tx	RS232 PRINTER	RS232 serial link
						Tx Printer		2	Rx		
●	EMBEDDED COMPUTING				3x0.34 sh.	0V		3	0V	RS232	Connect the shielding
						Rx E.C.		4	Tx		
						Tx E.C.		5	Rx		
●	EMBEDDED COMPUTING					Rx		9	+	BUS RS485	
						Tx		10	-		
●	TURBINE TRANSMITTER EMA	C1	1/2"NPT	●	ADR 4x0.34 sh.	12V	Jn	11	12V	METERING INPUT 1	Connect the shielding
						V1	Mr	12	V1		
						V2	Vt	13	V2		
						0V	Bc	14	0V		
						12V		19	12V		
●	ADDITIVE METERING INPUT OR ADDITIVE READY					V1		20	V1	METERING INPUT 2	Connect the shielding
						0V		21	0V		
						+	Jn	33	+		
●	Pt100 TEMPERATURE PROBE			●	ADR 3x0.6 sh.	-	Bc	34	-	Pt100	Connect the shielding
						-	Vt	35	-		

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY

THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION

	INSTALLATION GUIDE DI 015 ENE GRAVITRONIQUE	Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C
		This document is available at www.alma-alma.fr

EQUIPMENTS CONNECTED TO THE MICROCOMPT+							INTERFACE POWER SUPPLY BOARD			
Option	Equipement	Cable (for information)				Function	Colour or No.	Terminal	Function	Observation
		No.	CG*	Alma	Type					
GRAVITRONIQUE CONTROL BOX	C3	3/4"NPT	20x1			Pump	1	73	FET=Field Effect Transistor Outputs 24VDC (outputs FET 24V 5W max.)	Selection valve pumped distribution
						Gravi	2	79		Selection valve gravity distribution (in case of a double-stage API adaptor, Low Flow is operated with the gravity output control)
						Footvalve	3	44		Footvalve
						Vent	4	45		Vent
						Flap 1	5	39		Manifold vent control
						Flap 2	6	40		Opening-control flap 1
						Flap 3	7	41		Opening-control flap 2
						Flap 4	8	42		Opening-control flap 3
						Flap 5	9	43		Opening-control flap 4
						Return 1	10	63		Opening-control flap 5
						Return 2	11	64		Opening-control return 1
						Return 3	12	65		Opening-control return 2
						Return 4	13	66		Opening-control return 3
						Return 5	14	67		Opening-control return 4
						Declutching	15	62		Opening-control return 5
						Blowing	16	68	Declutching Blowing	Pump declutching or Motor acceleration (if automatic transmission)
						Hose 1	17	76		Product return blowing
						Hose 2	18	77	Valve hose 1/ EV manifold flap 6 Valve hose 2 / Product Return 6	Selection valve hose 1 (pumped) or Opening-control flap 6
						HF	19	78		Selection valve hose 2 (pumped) or Opening-control return 6
						LF	20	79	API	High flow of an API adaptor or Selection valve hose 3 (pumped) or Special return
										Low flow of an API adaptor
•	RC-HEATING OIL RECEIVER			2x1	Start/Stop	1	49	Start/Stop	RC-Oil_1	
•	OVERFILL PROTECTION (customer tank)				LF/HF	2	50	LF/HF	RC-Oil_2	
•	FLAP-CONTROL FEEDBACK						53			Overfill protection probe (customer tank)
•	PTO CONTROL			1x1	PTO Ctrl		58		PTO control	Power-take-off engaged
•	DRIVER'S CAB CONTROL			3x1	PTO	4	61	24VDC=PTO	PTO	(Output FET 24V 5W max.) FET=Field Effect Transistor
•	ADDITIONAL CONTROL			2x1	Supply	1	71	NC free contact	Additionnal control	Closed contact=additional (Output: NO free potential relay)
KIT SOLENOID VALVES NC/NO (ATEX) - PUMP BYPASS	C4		3xG0.75	Control	2	72				
					NC valve Pump bypass	1 / Mr	74	24VDC	NC or HF	24VDC = opening NC solenoid valve or HF control
					2 / Bl	80	0V			
				NO valve Exhaust	1 / Mr	75	24VDC	NO or LF		24VDC = closing NO solenoid valve or LF control

SOME EXTENSION BOARDS MAY BE SET ON TO THE INTERFACE POWER SUPPLY BOARD

*Refer to the Cable Glands Installation Instruction

Factory pre-wiring:

Cable (for information)							INTERFACE POWER SUPPLY BOARD			
Option	Equipment	Cable (for information)				Function	Colour or No.	Terminal	Function	Observation
		No.	CG*	Alma	Type					
	EXTENSION BOARD 4-RELAYS					Motor control		22	Start Mot. Stop Mot.	To extention board 4-relais


ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY

THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION

	INSTALLATION GUIDE DI 015 ENE GRAVITRONIQUE	Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C
		This document is available at www.alma-alma.fr

Terminal assignment of the extension board 4DG (IS)


EXTENSION BOARD 4DG (IS)

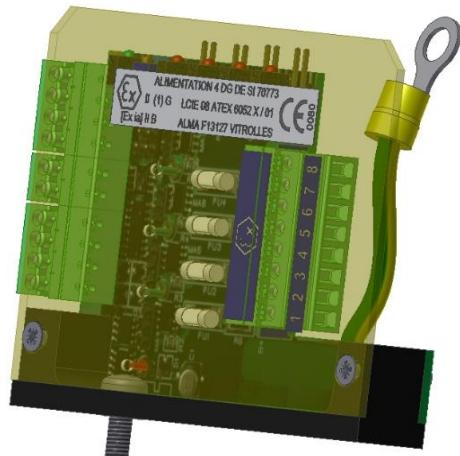

NT IN ATEX 506 C

EQUIPMENTS CONNECTED TO THE MICROCOMPT+							EXTENSION BOARD 4DG (IS)			
Option	Equipment	Cable (for information)				Function	Colour or No.	Terminal	Function	Observation
		No.	CG*	Alma	Type					
	END-OF-METERING PROBE				3x0.34	EMP	Mr	1	+	Connect the shielding
							Bl	2	-	
	VACUITY SENSOR				3x0.34	VACUITY	Mr	3	+	Connect the shielding
							Bl	4	-	
	DIFFERENTIAL PRESSURE TRANSMITTER				ADR 2x0.34 sh.	PRESSURE	Bc	5	+	Connect the shielding
							Mr	6	-	

*Refer to the Cable Glands Installation Instruction

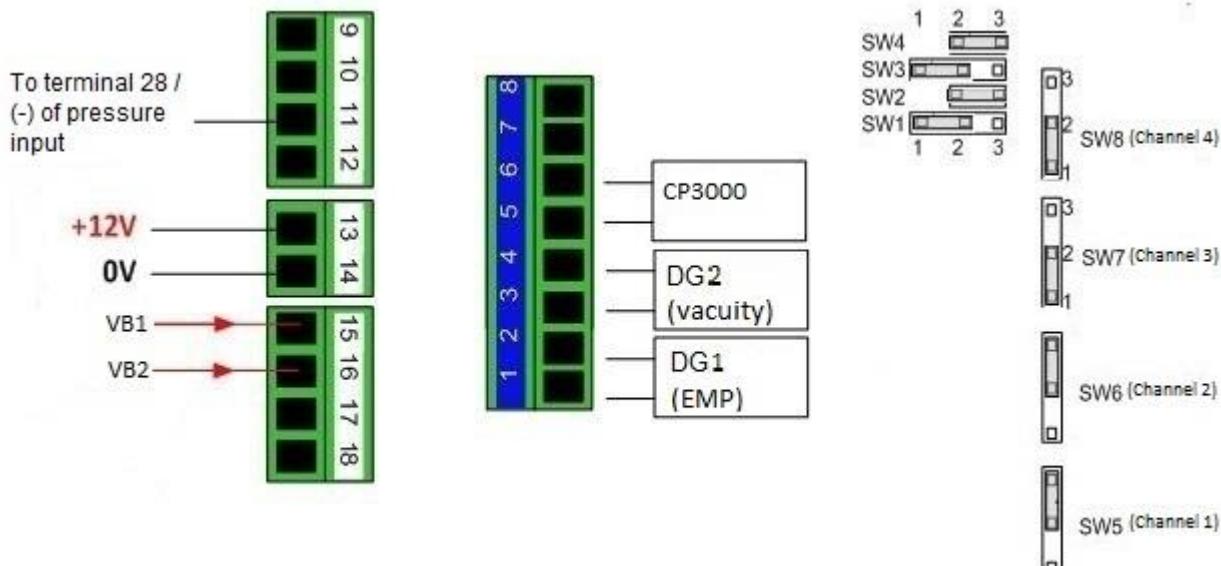Jumper configuration on the extension board 4DG:

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY

THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION

	INSTALLATION GUIDE DI 015 ENE GRAVITRONIQUE	Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C
	This document is available at www.alma-alma.fr	Page 18 / 47

Terminal assignment of the extension board 'sonde AD' 5wires (IS)

EXTENSION BOARD SONDE AD 5 wires (IS)




NT IN ATEX 510 C

EQUIPEMENTS CONNECTED TO THE MICROCOMPT+							EXTENSION BOARD SONDE AD (IS)			
Option	Equipement	Cable (for information)				Function or No.	Terminale	Function		Observation
		No.	CG*	Alma	Type					
	OVERFILL PROTECTION PROBE PLUG		[6x1]			Common	[Nr]	1	-	OVERFILL PROTECTIO N PROBES
						Supply	[Rg]	2	+	
						From probe	[Or]	3	From probe	
						To probe	[Jn]	4	To probe	

*Refer to the Cable Glands Installation Instruction

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY		
THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION		
	INSTALLATION GUIDE DI 015 ENE GRAVITRONIQUE	Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C
This document is available at www.alma-alma.fr		Page 19 / 47

Terminal assignment of the relay extension board

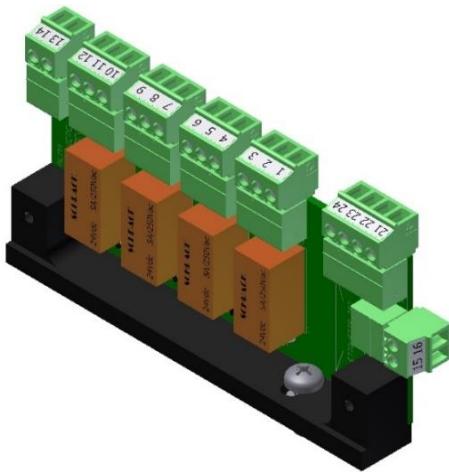RELAY EXTENSION BOARD (used to control a minimum 5W spool valve)										
										
EQUIPEMENT CONNECTED TO THE MICROCOMPT+							RELAY EXTENSION BOARD			
Option	Equipement	Cable (for information)				Function	Colour or No.	Terminal	Function	
		No.	CG*	Alma	Type					
•	DRIVER' CAB CONTROL	3x1				Start engine		1	NC	Start engine
								2	Common	
								3	NO	
		3x1				Stop engine		4	NC	Stop engine
								5	Common	
								6	NO	

*Refer to the Cable Glands Installation Instructions

Factory pre-wiring:


INTERFACE POWER SUPPLY BOARD							EXTENSION BOARD 4-RELAIS				Observation	
Option	Equipment	Cable (for information)				Function	Colour or No.	Terminal	Function			
		No.	CG*	Alma	Type							
	POWER SUPPLY					Supply	Bl	15	24VDC	Supply		
						Mass	N	16	0V			
	MOTOR CONTROL					Engine control	22	21		Engine control		
							23	22				



On the extension board 4-relais, cut the diodes D3 and D4 off.


ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY		
THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION		
	INSTALLATION GUIDE DI 015 ENE GRAVITRONIQUE	Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C
This document is available at www.alma-alma.fr		Page 20 / 47

Control box GRAVITRONIQUE

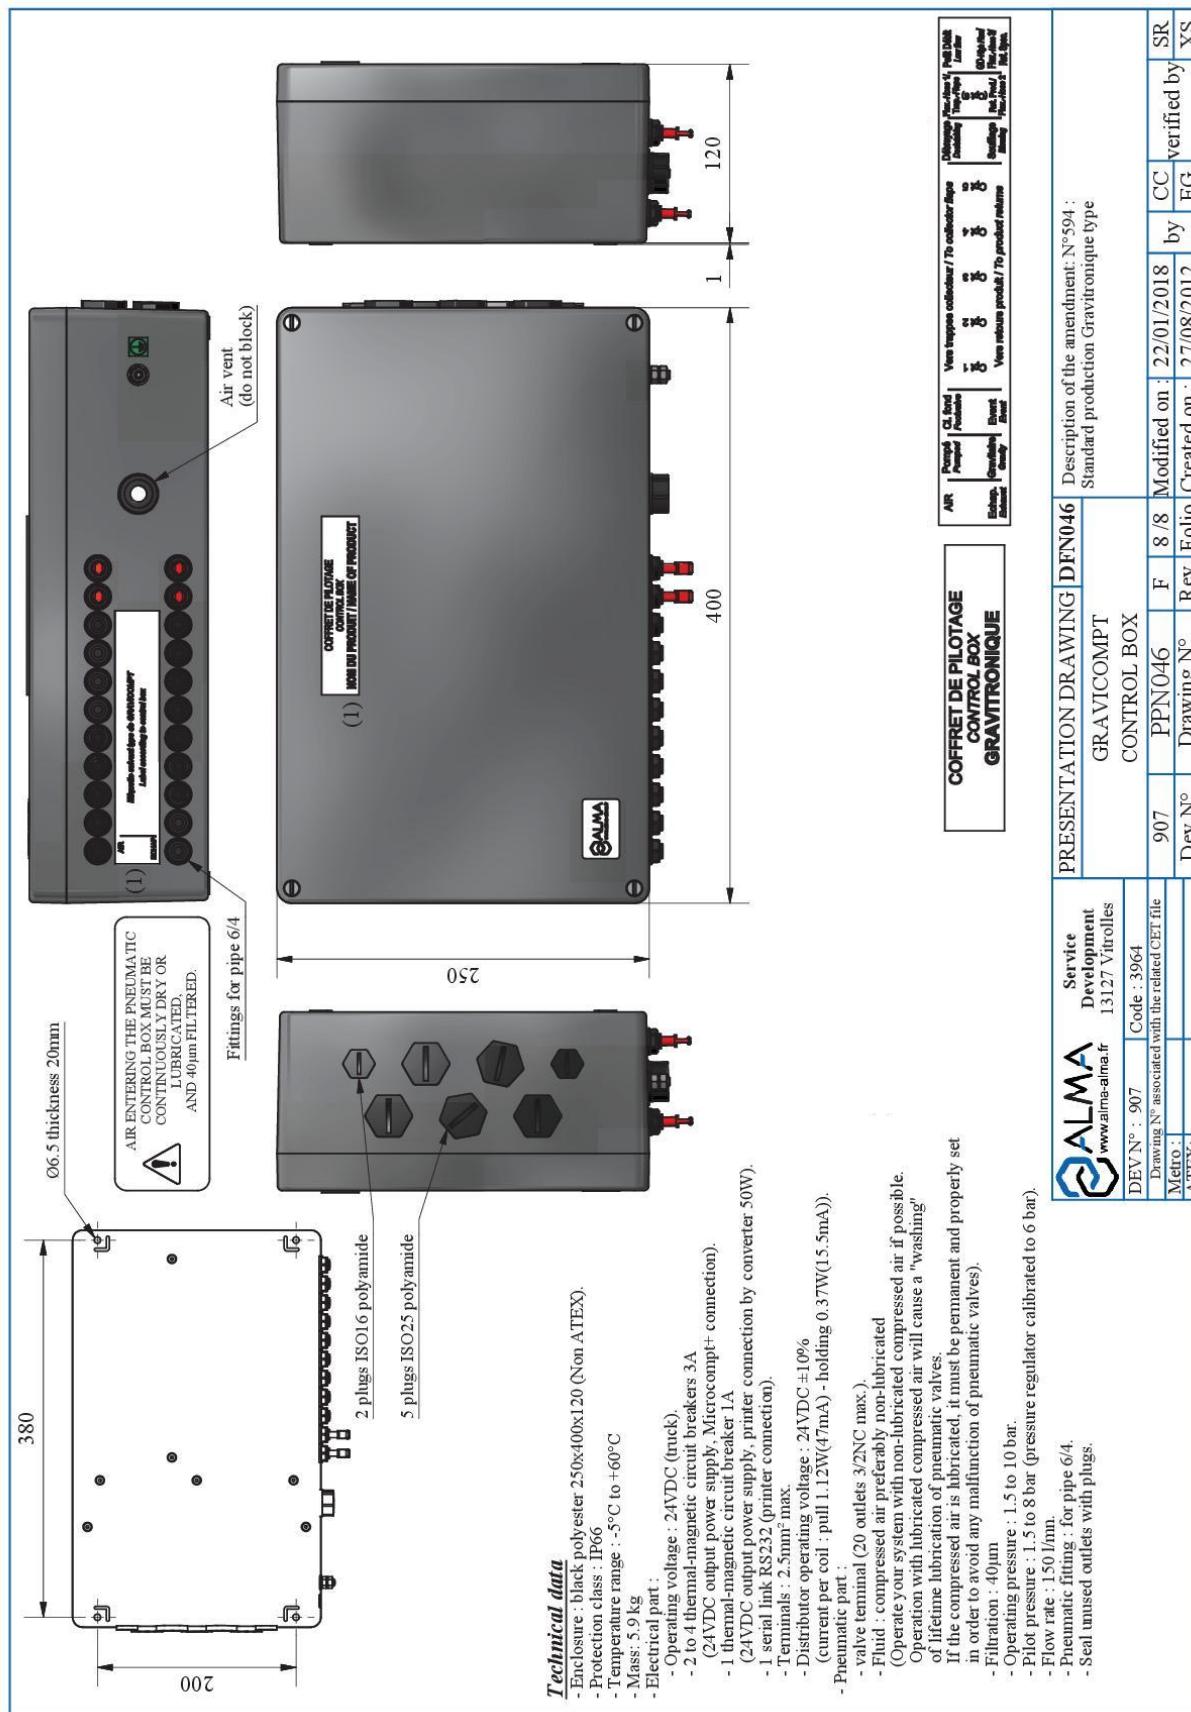

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY			
THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION			
	INSTALLATION GUIDE DI 015 EN E GRAVITRONIQUE		Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C
	This document is available at www.alma-alma.fr		

Document available on website [alma-alma.fr](http://www.alma-alma.fr)

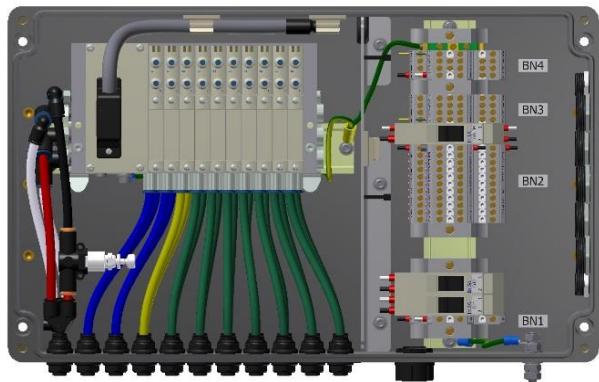Electrical wiring control box**TERMINAL ASSIGNMENT OF CONTROL BOX**

EQUIPMENTS CONNECTED TO THE CONTROL BOX							CONTROL BOX TERMINAL BLOCKS					
Option	Equipement	Cable (for information)				Fnction	Colour or No.	Block	Terminal	Function	Observation	
		No.	CG*	Alma	Type							
	SUPPLY	A1			2x1	24VDC	1	BN1	1	24VDC	Supply	24VDC truck battery (after battery switch and protected by a fuse)
						0V	2		2	0V		
	MICROCOMPT+	C3	3/4"NPT		20x1	24VDC	2		1	Gravity		Selection valve gravity distribution (in case of a double- stage API adaptor, Low Flow is operated with the gravity output control)
						24VDC	4		3	Vent		Vent valve control
						24VDC	10		5	Return 1	Product return	Product return 1 to 5
						24VDC	11		7	Return 2		
						24VDC	12		9	Return 3		
						24VDC	13		11	Return 4		
						24VDC	14		13	Return 5		
						24VDC	16		15	Blowing		Product return blowing
						24VDC	18		17	Hose 2 / Return 6		Selection valve hose 2 (pumped) or product return compartment 6
						24VDC	19		19	HF / Hose 3 / Special return		High flow of an API adaptor or Selection valve hose 3 (pumped) or Special return
						24VDC	1		2	Pump		Selection valve pumped distribution
						24VDC	3		4	Footvalve		Footvalve control
						24VDC	5		6	Flap 1	Flap opening	Flap control compartments 1 to 5
						24VDC	6		8	Flap 2		
						24VDC	7		10	Flap 3		
						24VDC	8		12	Flap 4		
						24VDC	9		14	Flap 5		
						24VDC	15		16	Declutch.		Pump declutching or Motor acceleration
						24VDC	17		18	Hose 1 / Flap 6		Selection valve hose 1(pumped) or Flap control compartment 6
						24VDC	20		20	Low flow	LF	Lox flow of an API adaptor (in case of a double- stage API adaptor, Low Flow is operated with the gravity output control)

*Refer to the Cable Glands Installation Instructions

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY

THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION

	INSTALLATION GUIDE DI 015 ENE GRAVITRONIQUE	Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C
		This document is available at www.alma-alma.fr

EQUIPMENTS CONNECTED TO THE CONTROL BOX							CONTROL BOX TERMINAL BLOCKS				
Option	Equipment	Cable (for information)				Function	Colour or No.	Block	Terminal	Function	Observation
		No.	CG*	Alma	Type						
	MICROCOMPT+	C2				+	Bl	DJ1		Microcompt supply	
	MICROCOMPT+					-	N				
	MICROCOMPT+					Rx		Bn3	8	Printer supply	
	MICROCOMPT+					Tx			7		
	PRINTER		1/2"NPT		4x1 sh.	+	Bl	Bn4	1		
	PRINTER					-	N		2	Input	Converter
	PRINTER					0V	Vt		6	0V	
	PRINTER					Rx	Bc		7	Rx	Printer RS232 serial link
	PRINTER					Tx	Mr		8	Tx	

*Refer to the Cable Glands Installation Instructions

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY		
THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION		
	INSTALLATION GUIDE DI 015 ENE GRAVITRONIQUE	Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C
	This document is available at www.alma-alma.fr	Page 23 / 47

Pneumatic wiring control box**PNEUMATIC INPUT/OUTPUT ASSIGNMENT OF THE CONTROL BOX**

Label	Input	Output	Function	Observation
AIR	X		Air supply of the box	Air if: all footvalves opened and valve bar locked
Exhaust		X	Exhaust	Put a tube L=100mm min. (no muffler)
Pumped	X		Pumped way selection	
Gravity	X		Gravity way selection	
Footvalve	X		Opening footvalve	
Vent	X		Opening manifold vent	Connection to the vent valve
Collector flap Cpt 1	X		Opening flaps compartments 1 to 5	Connection to the manifold flaps compartments 1 to 5
Collector flap Cpt 2	X			
Collector flap Cpt 3	X			
Collector flap Cpt 4	X			
Collector flap Cpt 5	X			
Product return Cpt 1	X		Product returns compartments 1 to 5	Connection to the product returns compartments 1 to 5
Product return Cpt 2	X			
Product return Cpt 3	X			
Product return Cpt 4	X			
Product return Cpt 5	X			
Declutching	X		Declutching pneumatic cylinder	If pneumatic declutching
Blowing	X		Product return blowing	Use "&" cells to connect with each return product control
Hose 1/ Collector flap Cpt 6		X	Hose 1 valve control or Opening flap compartment 6	Connection to the product return compartment6
Hose 2/ Product return Cpt 6		X	Hose 2 valve control or Product return compartment 6	Connection to the manifold flap compartment 6
Low Flow		X	API adaptor open in low flow	Connection to the API adaptor (HF – LF)
High Flow/ Hose 3/ Ret. Spec.		X	API adaptor open in high flow	

Unused ports must be plugged.

**CONDITIONS FOR AIR SUPPLY OF THE CONTROL BOX:**

- The pneumatic "&" cells of all footvalves are open.
- The bar is in its locked position (compartment API adapters are locked).


ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY

THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION

	INSTALLATION GUIDE DI 015 EN E GRAVITRONIQUE	Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C
	This document is available at www.alma-alma.fr	Page 24 / 47

6. ADRIANE TURBINE METER

6.1. TURBINE METER ADRIANE DN100-80 243 TTMA WITH SIGHTGLASS

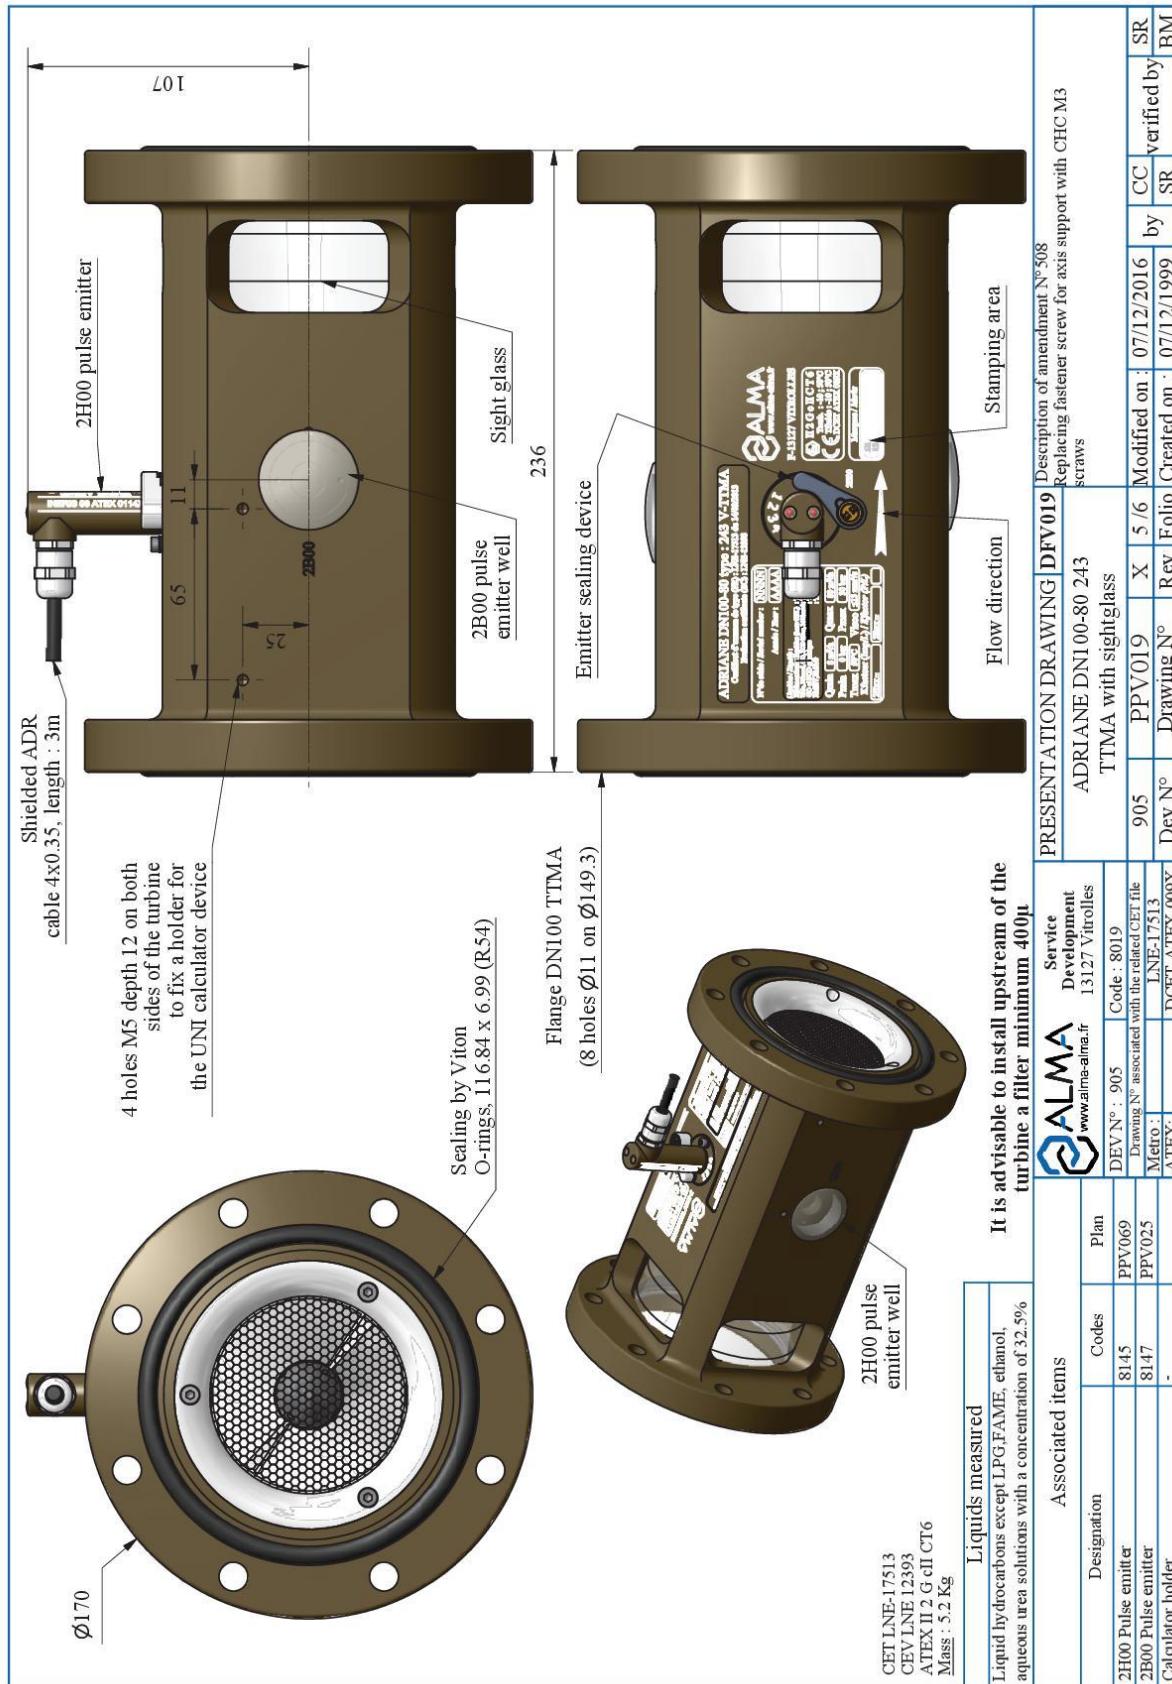

Document available on website alma-alma.fr

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY

THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION




INSTALLATION GUIDE DI 015 EN E GRAVITRONIQUE

This document is available at www.alma-alma.fr

Page 25 / 47

6.2. TURBINE ADRIANE DN80-80 243 110x110

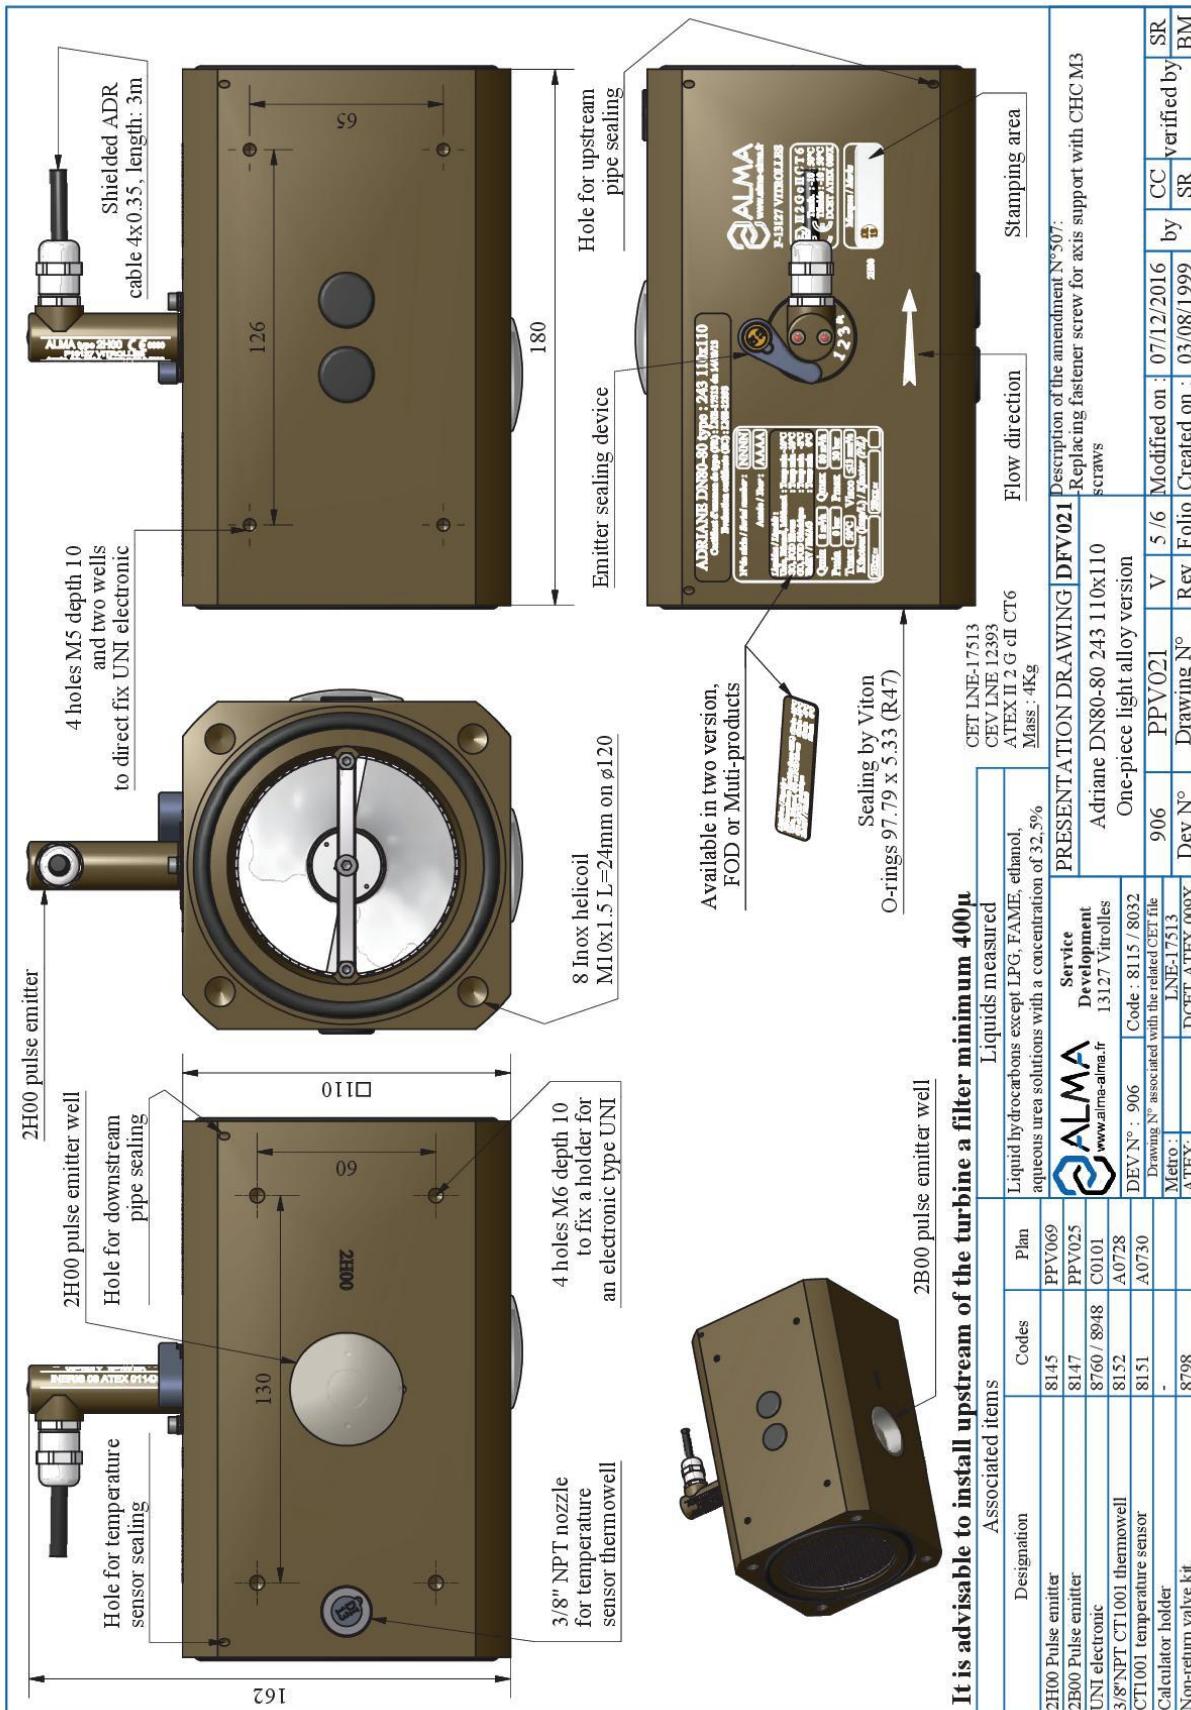


It is advisable to install upstream of the turbine a filter minimum 400 "

Document available on website alma-alma.fr

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY		
THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION		
	INSTALLATION GUIDE DI 015 EN E GRAVITRONIQUE	<u>Units of measure:</u> Length: mm Angle: degree (° ′ ″) Temperature: °C
	This document is available at www.alma-alma.fr	Page 26 / 47

6.3. INSTALLATION AND SEALING RECOMMENDATIONS ADRIANE TURBINE METER

- The identification plate and the led of the pulse emitter(s) shall be visible and accessible.
- The turbine must be installed with respect to the flow direction.
- Put sealing rings each other sides between the turbine and the backflanges.
- Leave an open space all around the turbine in order to ease maintenance.
- Install a 400 μ filter (mini) on the pipe upstream from the turbine meter.
- After installation or during the commissioning period, if the new or modified pipes have not been perfectly cleaned or pickled and passivated, the turbine should be protected by a honeycomb sieve – max. 1mm mesh. It must be placed between two flanges upstream from the turbine.
- Dimensions: A > 100mm.

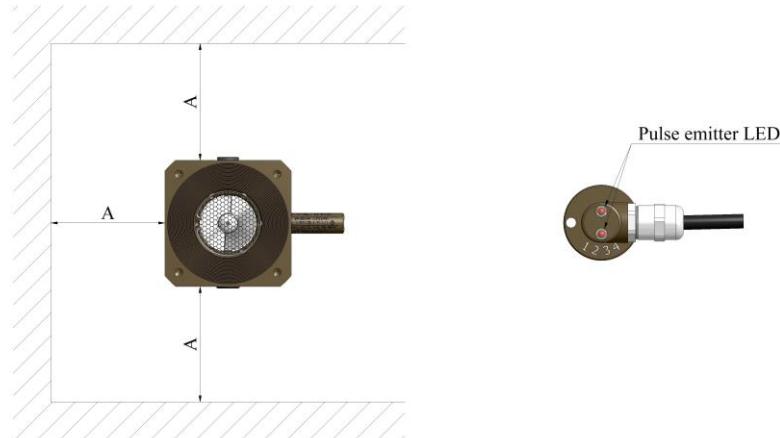

- Refer to the certificate written on the identification plate of the measuring system to suit the sealing requirements
- No loose lead wire on the sealing devices



For accuracy class 0.5 and 1.0 measuring systems, the pipes and equipment upstream or downstream the turbine meter must have the same nominal diameter as the meter on a length at least equal to 10 times this diameter upstream and 5 times this diameter downstream.

These lengths can be straight or bent.

It is mandatory that no flowrate adjustment device (e.g. a variable-opening valve) is located upstream at a distance less than 10 times the nominal diameter of the meter:


Provision contained in EU Type Examination or Evaluation Certificate.

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY

THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION

	INSTALLATION GUIDE DI 015 EN E GRAVITRONIQUE	Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C
	This document is available at www.alma-alma.fr	Page 27 / 47

7. DIFFERENTIAL PRESSURE TRANSMITTER CP3000 ATEX




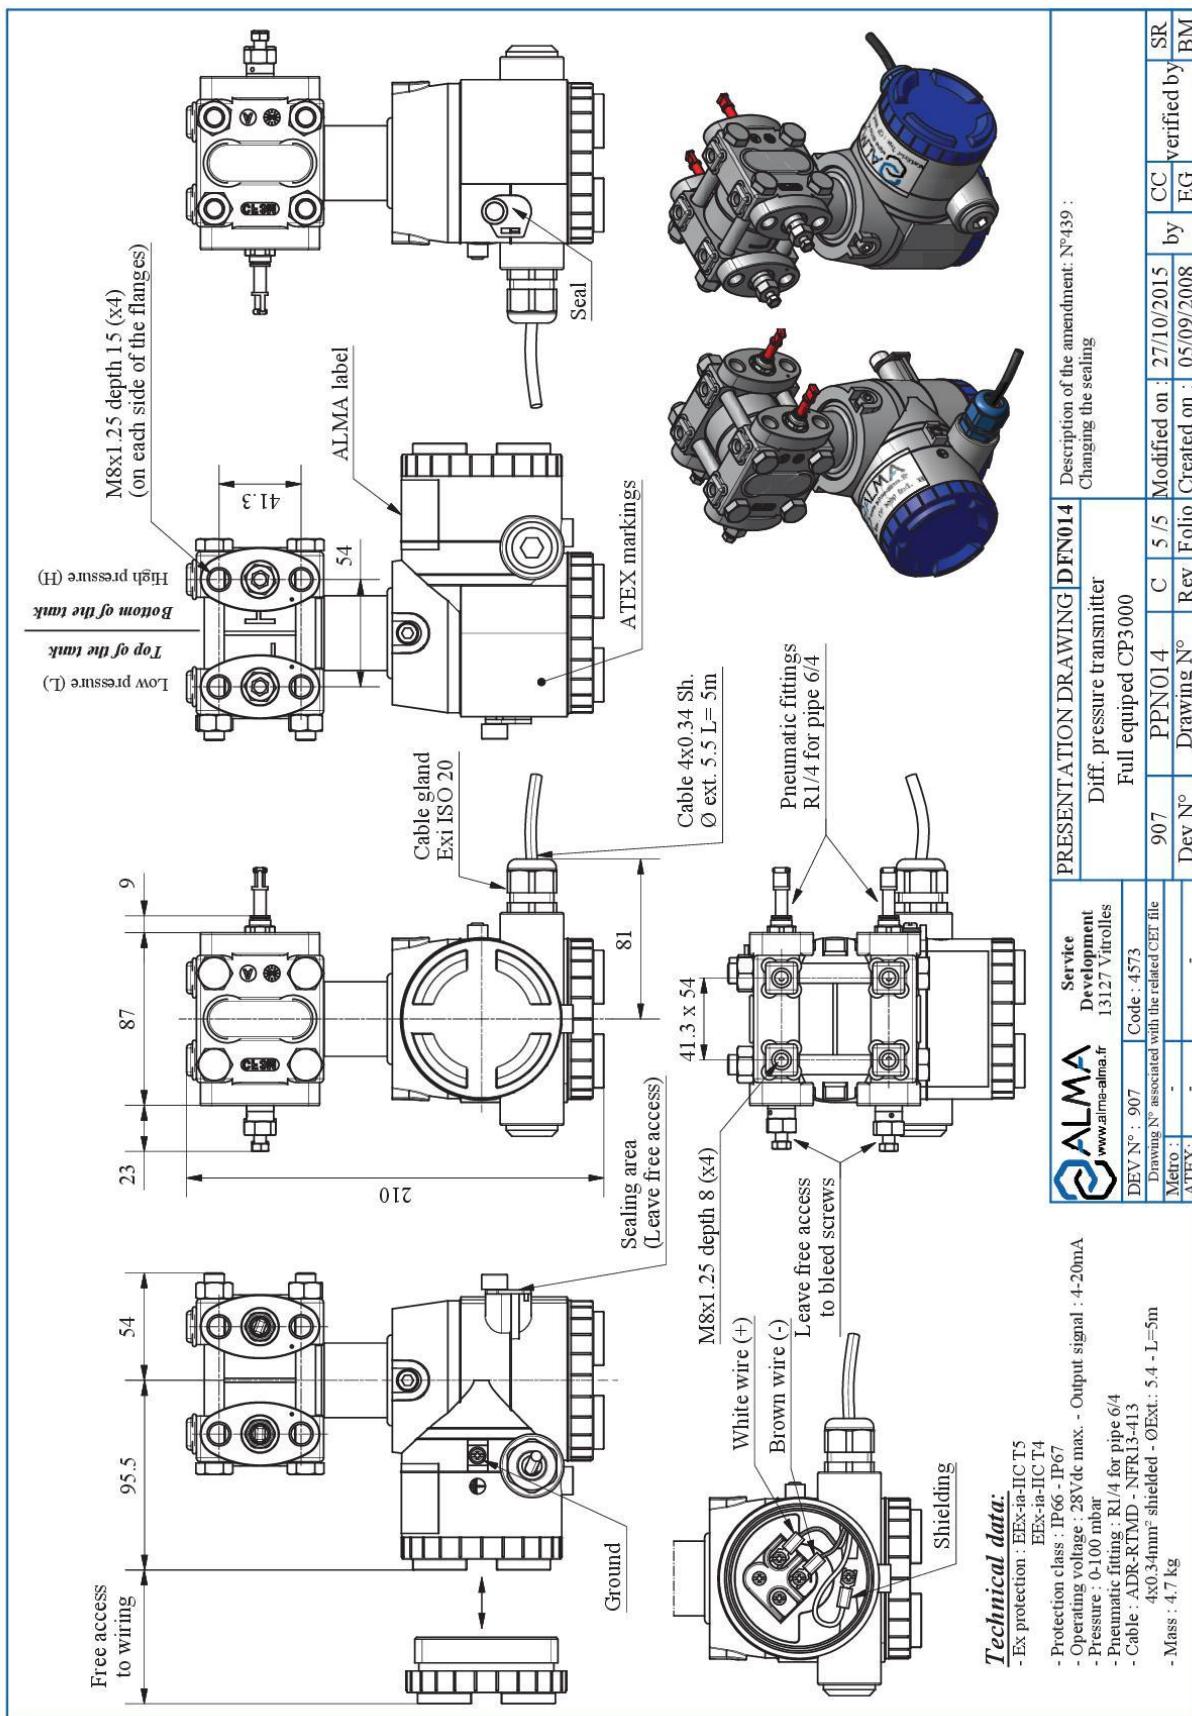


Document available on website [alma-alma.fr](http://www.alma-alma.fr)

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY			
THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION			
	INSTALLATION GUIDE DI 015 EN E GRAVITRONIQUE	Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C	
	This document is available at www.alma-alma.fr		Page 28 / 47

7.1. INSTALLATION RECOMMENDATIONS CP3000 ATEX


THE PRESSURE TRANSMITTER MUST BE INSTALLED IN UPRIGHT POSITION

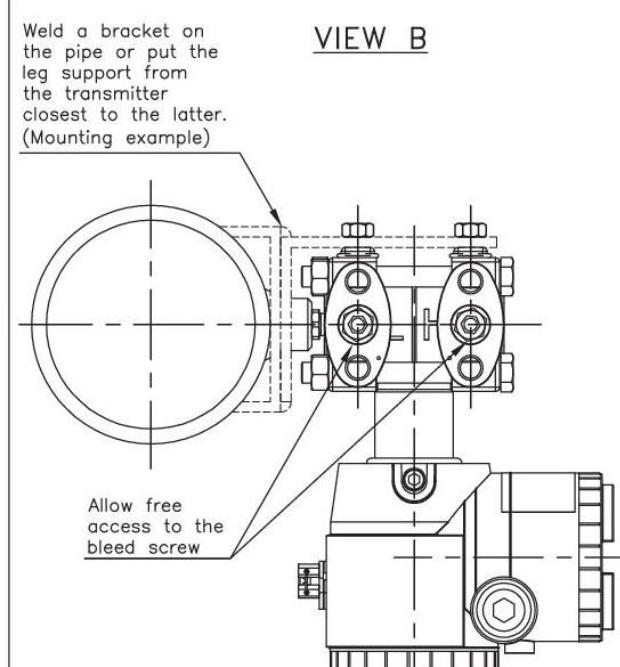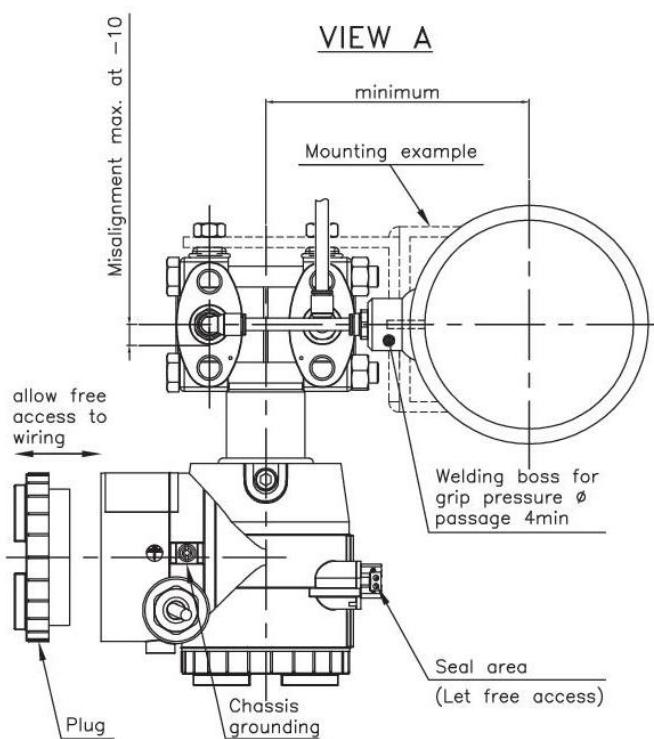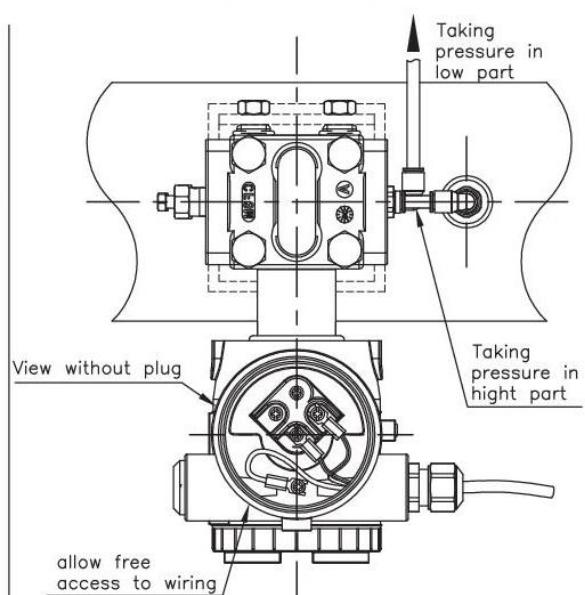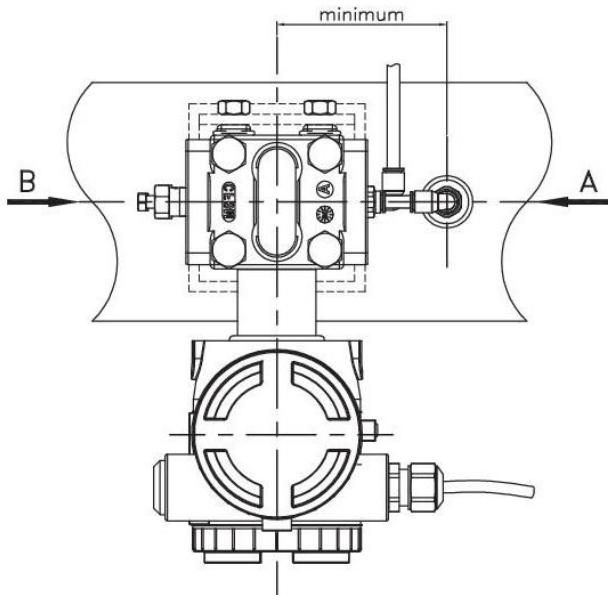

REFER TO INSTRUCTION MANUAL
(DELIVERED WITH THE EQUIPMENT AND AVAILABLE ON ALMA WEBSITE)

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY		
THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION		
	INSTALLATION GUIDE DI 015 EN E GRAVITRONIQUE	Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C
This document is available at www.alma-alma.fr		Page 29 / 47


8. NC/NO SOLENOID VALVES KIT ATEX

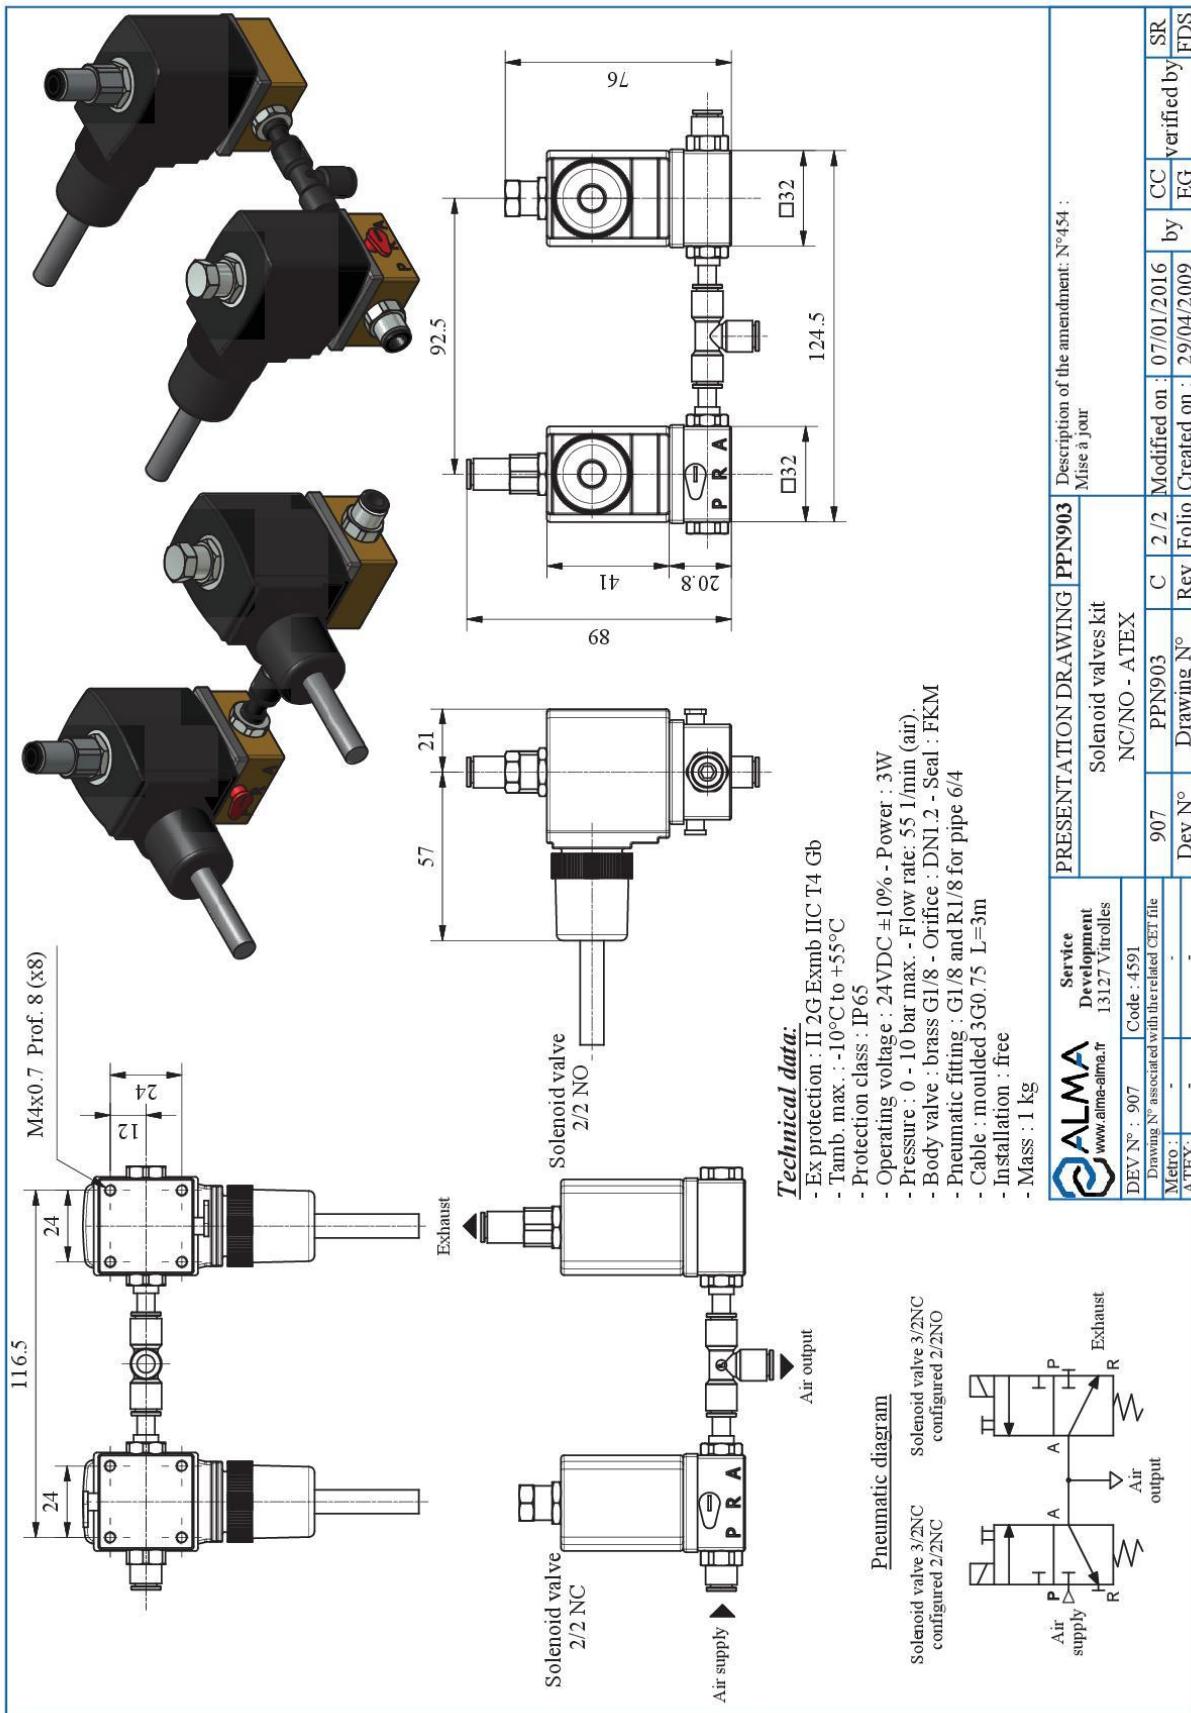

Document available on website alma-alma.fr

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY			
THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION			
	INSTALLATION GUIDE DI 015 EN E GRAVITRONIQUE	Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C	
	This document is available at www.alma-alma.fr		Page 30 / 47

9. END-OF-METERING PROBE / VACUITY SENSOR – DG3001/75

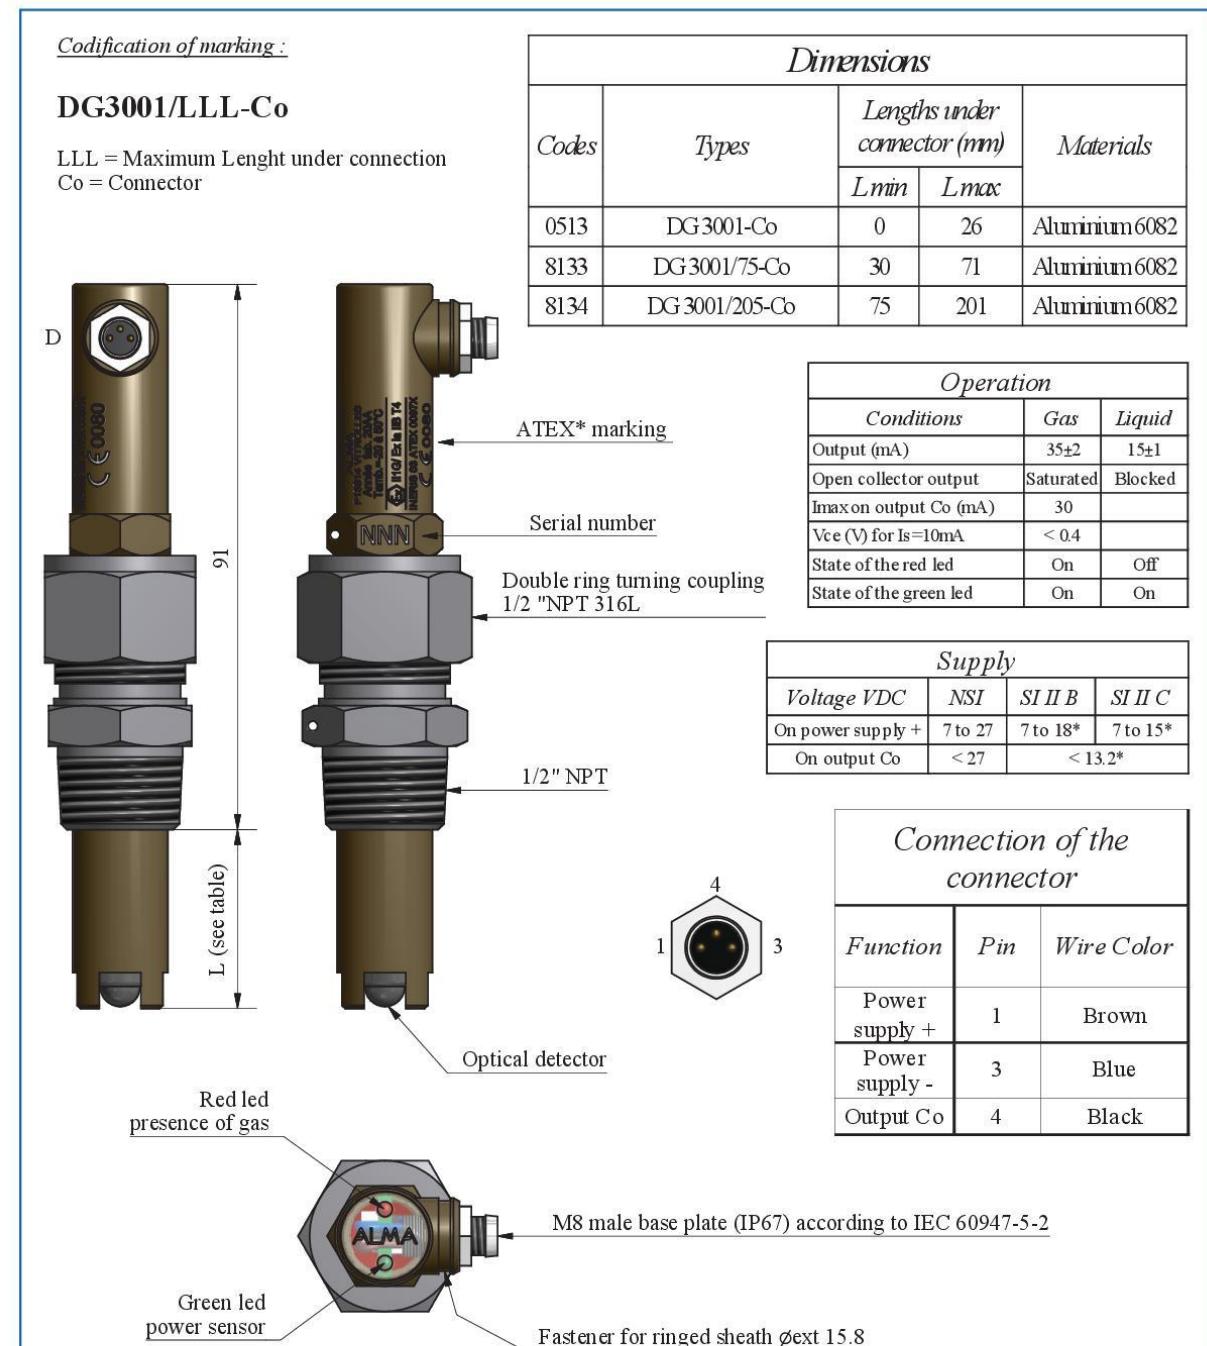


ALMA www.alma-alma.fr	Service Development 13127 Vitrolles	PRESENTATION DRAWING DFV014				Description of amendment N°522 Adding CI008 version 2 for DLA01		
		Gas detector output connector DG3001, DG3001/75, DG3001/205						
DEV N° : 981	Code : 0513	981	PPV014	V	6 / 8	Modified on : 22/12/2016	by CHR	verified by SR
Metro : ATEX:	Drawing N° associated with the related CET file INERIS 03 ATEX 0097X	Dev N°	Drawing N°	Rev	Folio	Created on : 01/04/1999	by SR	verified by BM

ALMA	ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY							
	THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION							
	INSTALLATION GUIDE DI 015 EN E GRAVITRONIQUE							
This document is available at www.alma-alma.fr		Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C						
		Page 31 / 47						

9.1. INSTALLATION RECOMMENDATIONS DG3001/75



POSITION OF THE END-OF-METERING AND VACUITY PROBES:

Location of the end-of-metering probe
(DG3001/75)

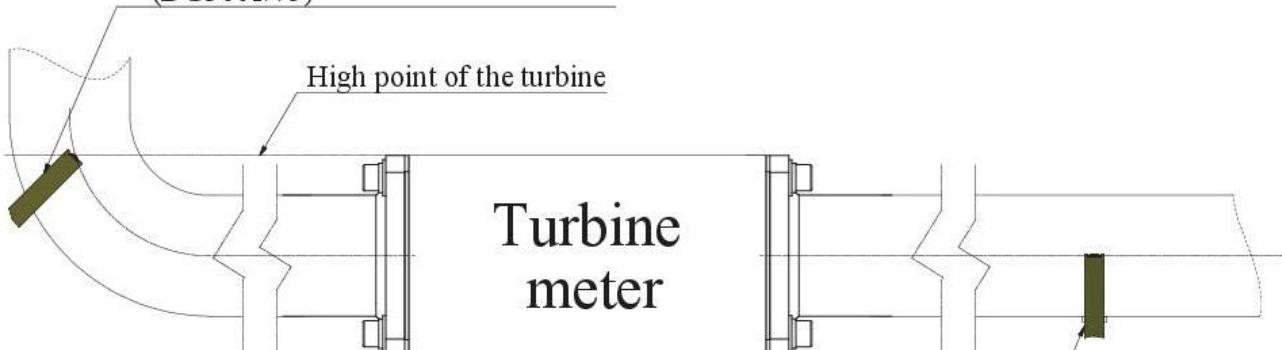

Location of the vacuity probe
(DG3001/75)

INSTALLATION OF THE END-OF-METERING AND VACUITY PROBES ON THE PIPE:

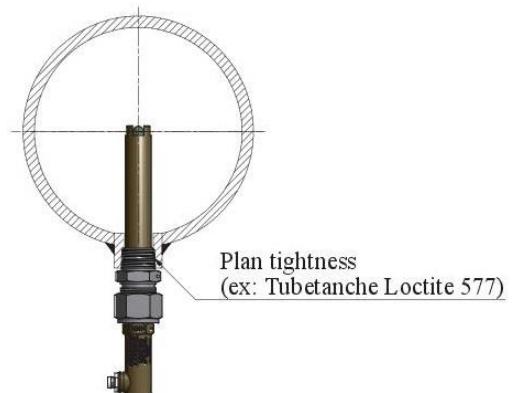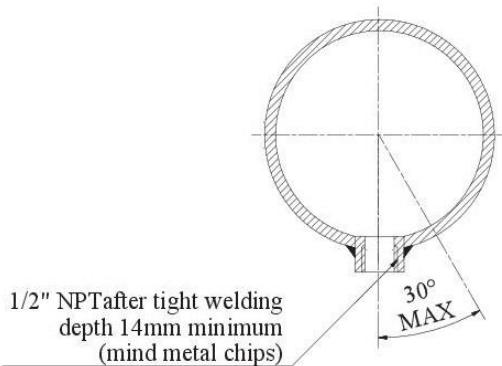

REFER TO INSTRUCTION MANUAL

(DELIVERED WITH THE EQUIPMENT AND AVAILABLE ON ALMA WEBSITE)

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY

THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION




INSTALLATION GUIDE DI 015 EN E
GRAVITRONIQUE

Units of measure:
Length: mm
Angle: degree (° ° °)
Temperature: °C

This document is available at www.alma-alma.fr

Page 32 / 47

10. PRINTER


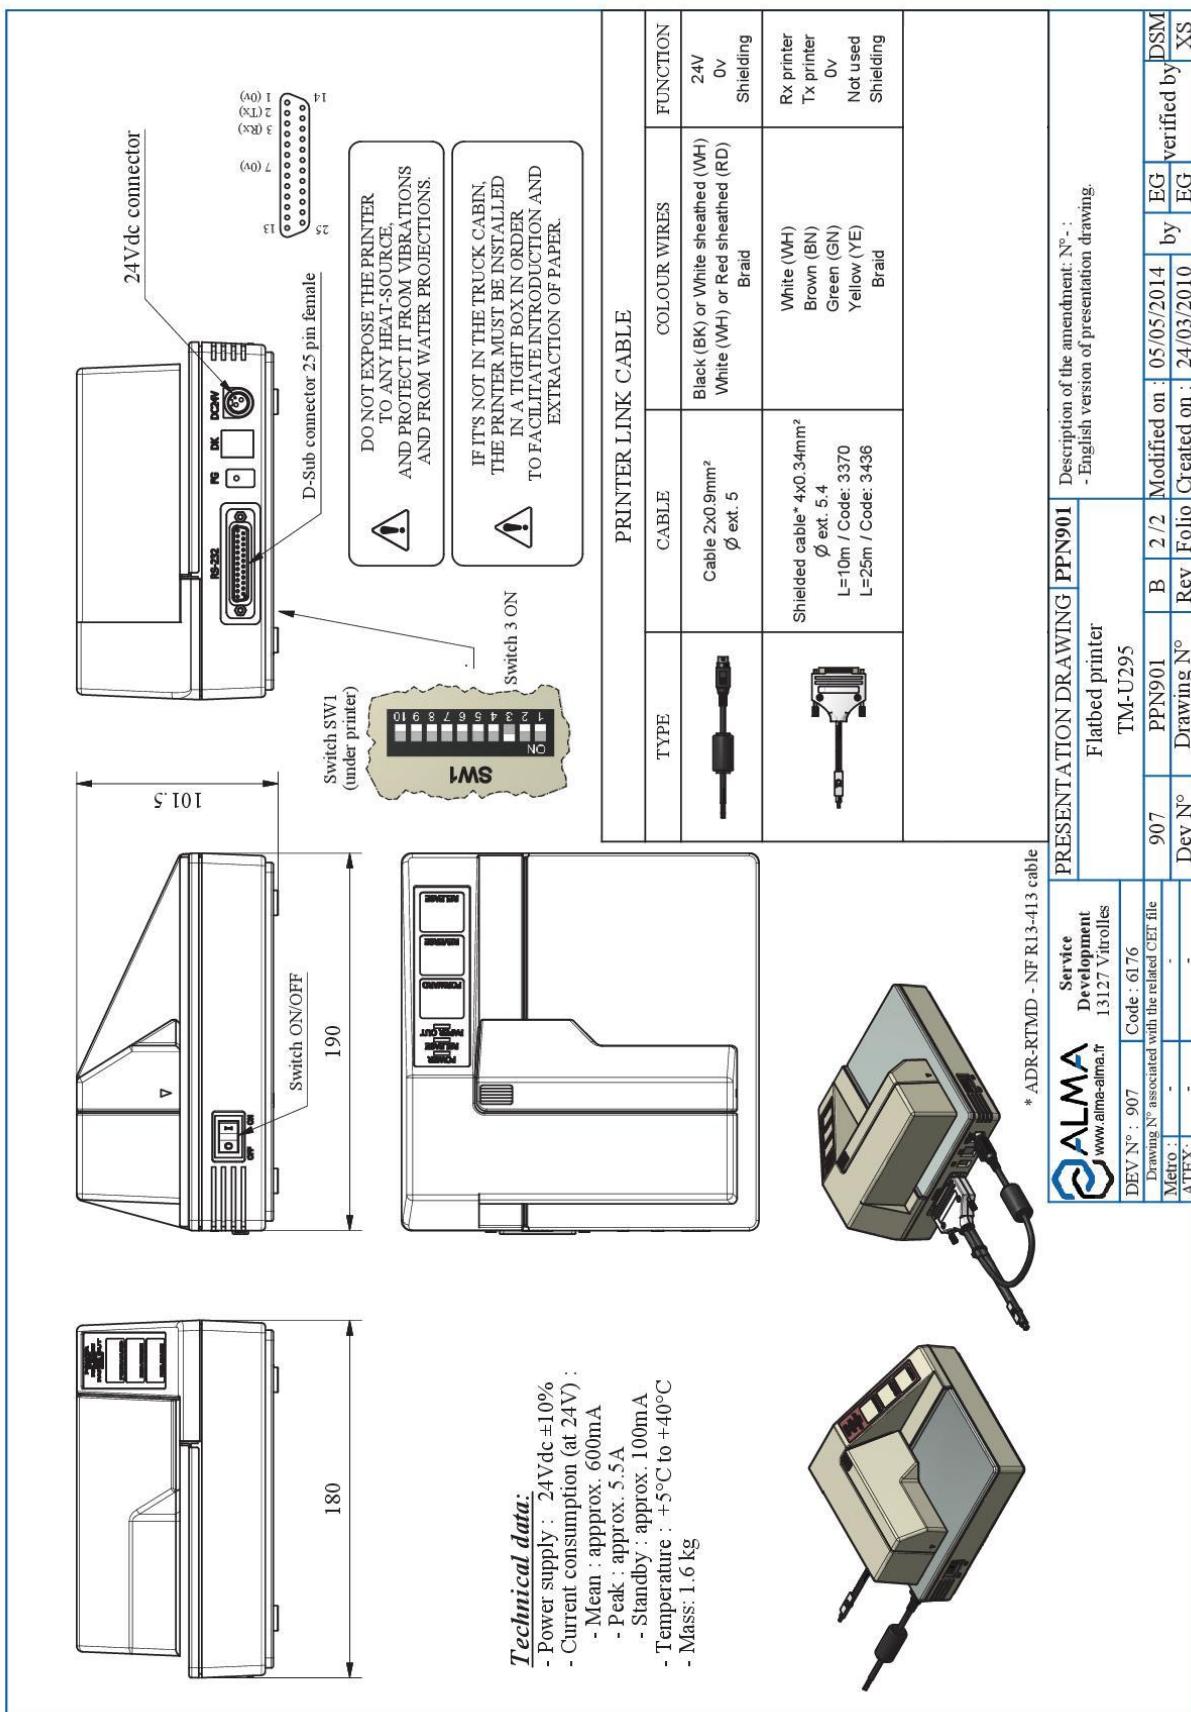


Document available on website alma-alma.fr

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY			
THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION			
	INSTALLATION GUIDE DI 015 ENE GRAVITRONIQUE	Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C	
This document is available at www.alma-alma.fr			Page 33 / 47

10.1. INSTALLATION RECOMMENDATIONS PRINTER

- The printer must be installed in a tight box and be laid out so as not to obstruct the introduction/extraction of sheet of paper (Dimension D).
- Do not store anything above the printer.
- Leave an open space all around the printer to ease maintenance.
- Dimensions: A ≥ 50mm, B ≥ 100mm, C ≥ 120mm.

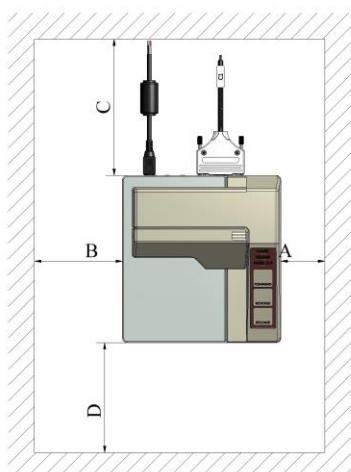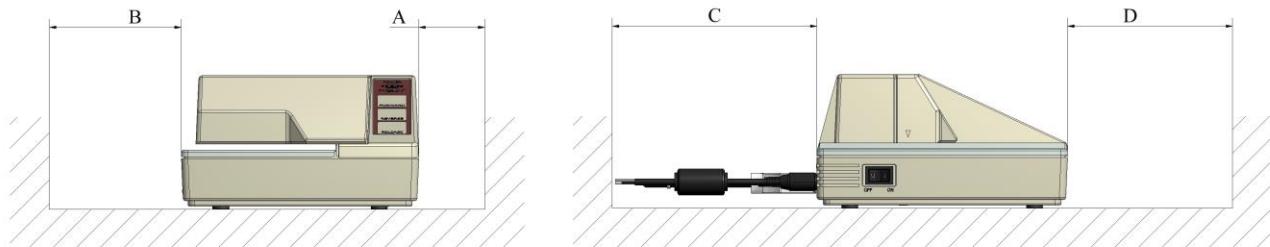

**DO NOT EXPOSE THE PRINTER TO ANY HEAT-SOURCE.
PROTECT IT FROM VIBRATIONS AND WATER PROJECTIONS.**

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY

THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION




**INSTALLATION GUIDE DI 015 EN E
GRAVITRONIQUE**

This document is available at www.alma-alma.fr

Units of measure:
Length: mm
Angle: degree (° ° °)
Temperature: °C

Page 34 / 47


11. CONVERTER 24VDC/24VDC 2.1A 50W

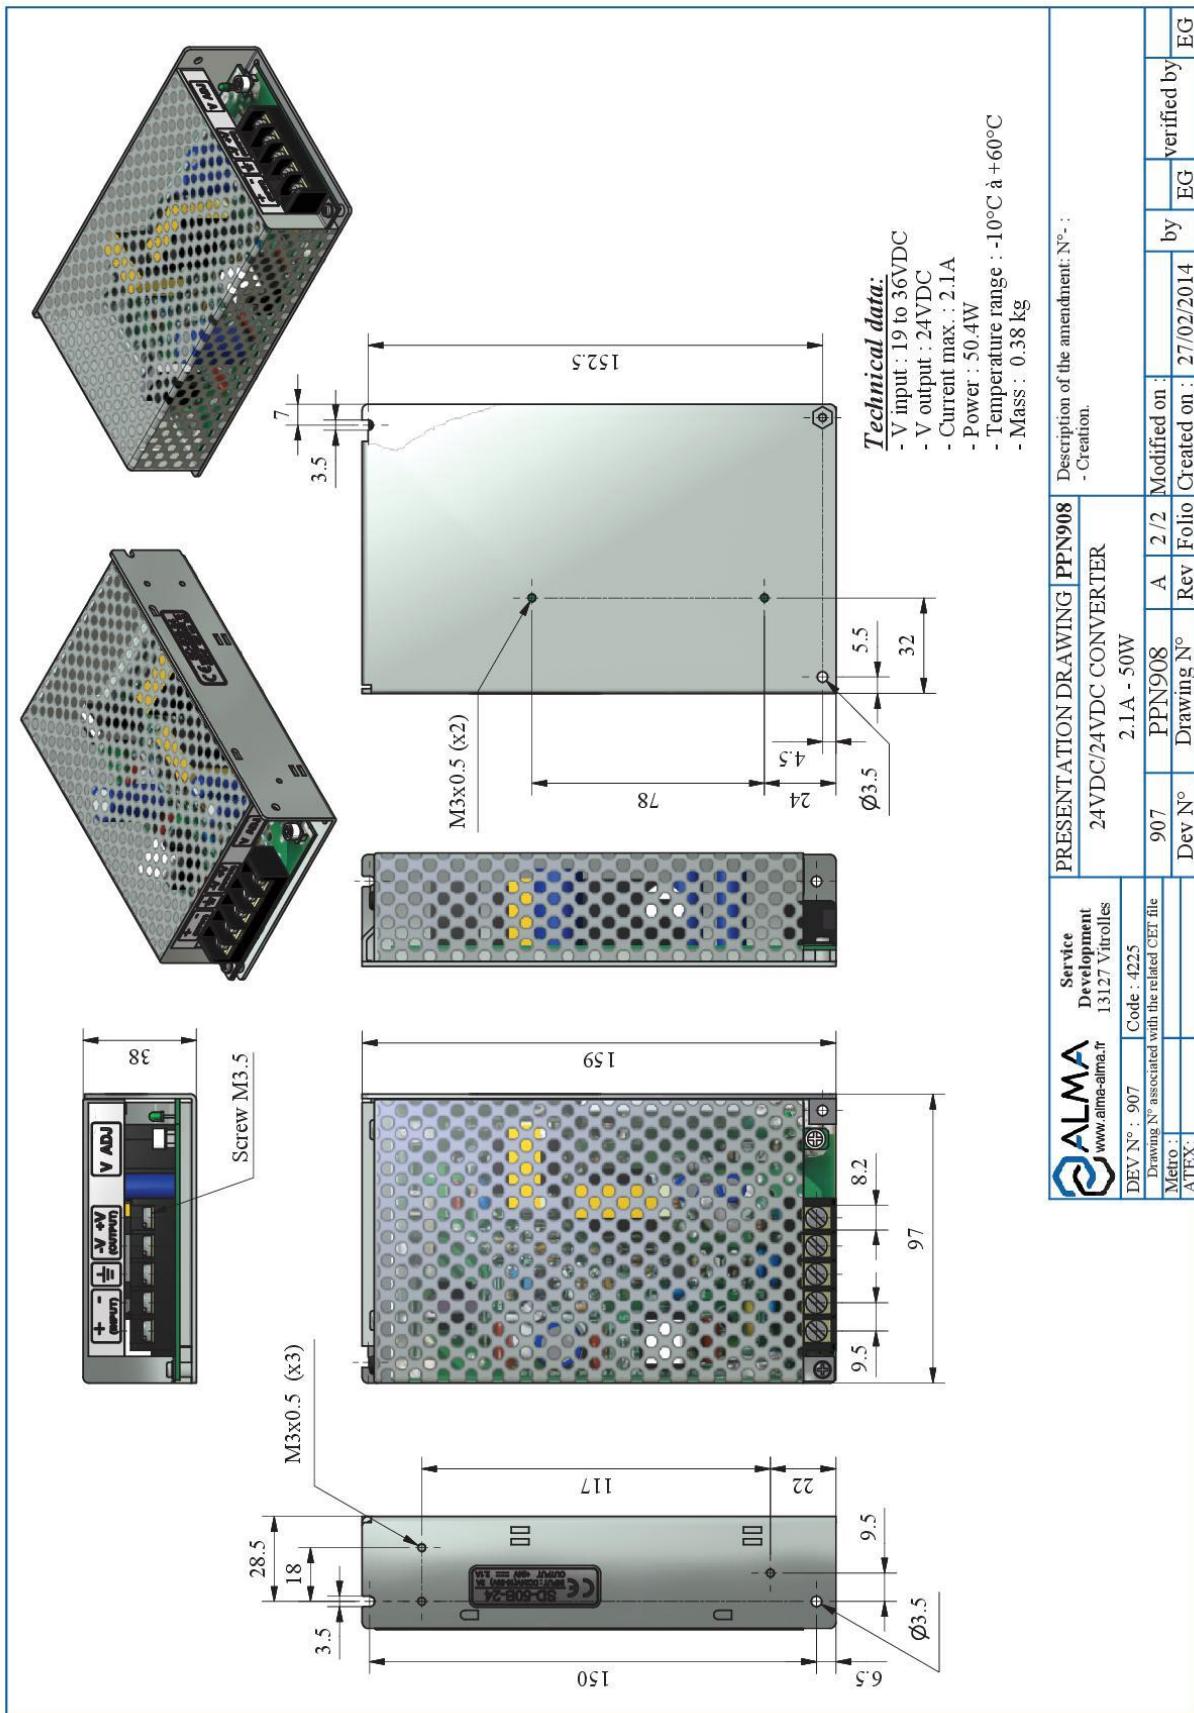

Document available on website [alma-alma.fr](http://www.alma-alma.fr)

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY		
THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION		
	INSTALLATION GUIDE DI 015 EN E GRAVITRONIQUE	Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C
This document is available at www.alma-alma.fr		Page 35 / 47

12. VACUUM BREAKER


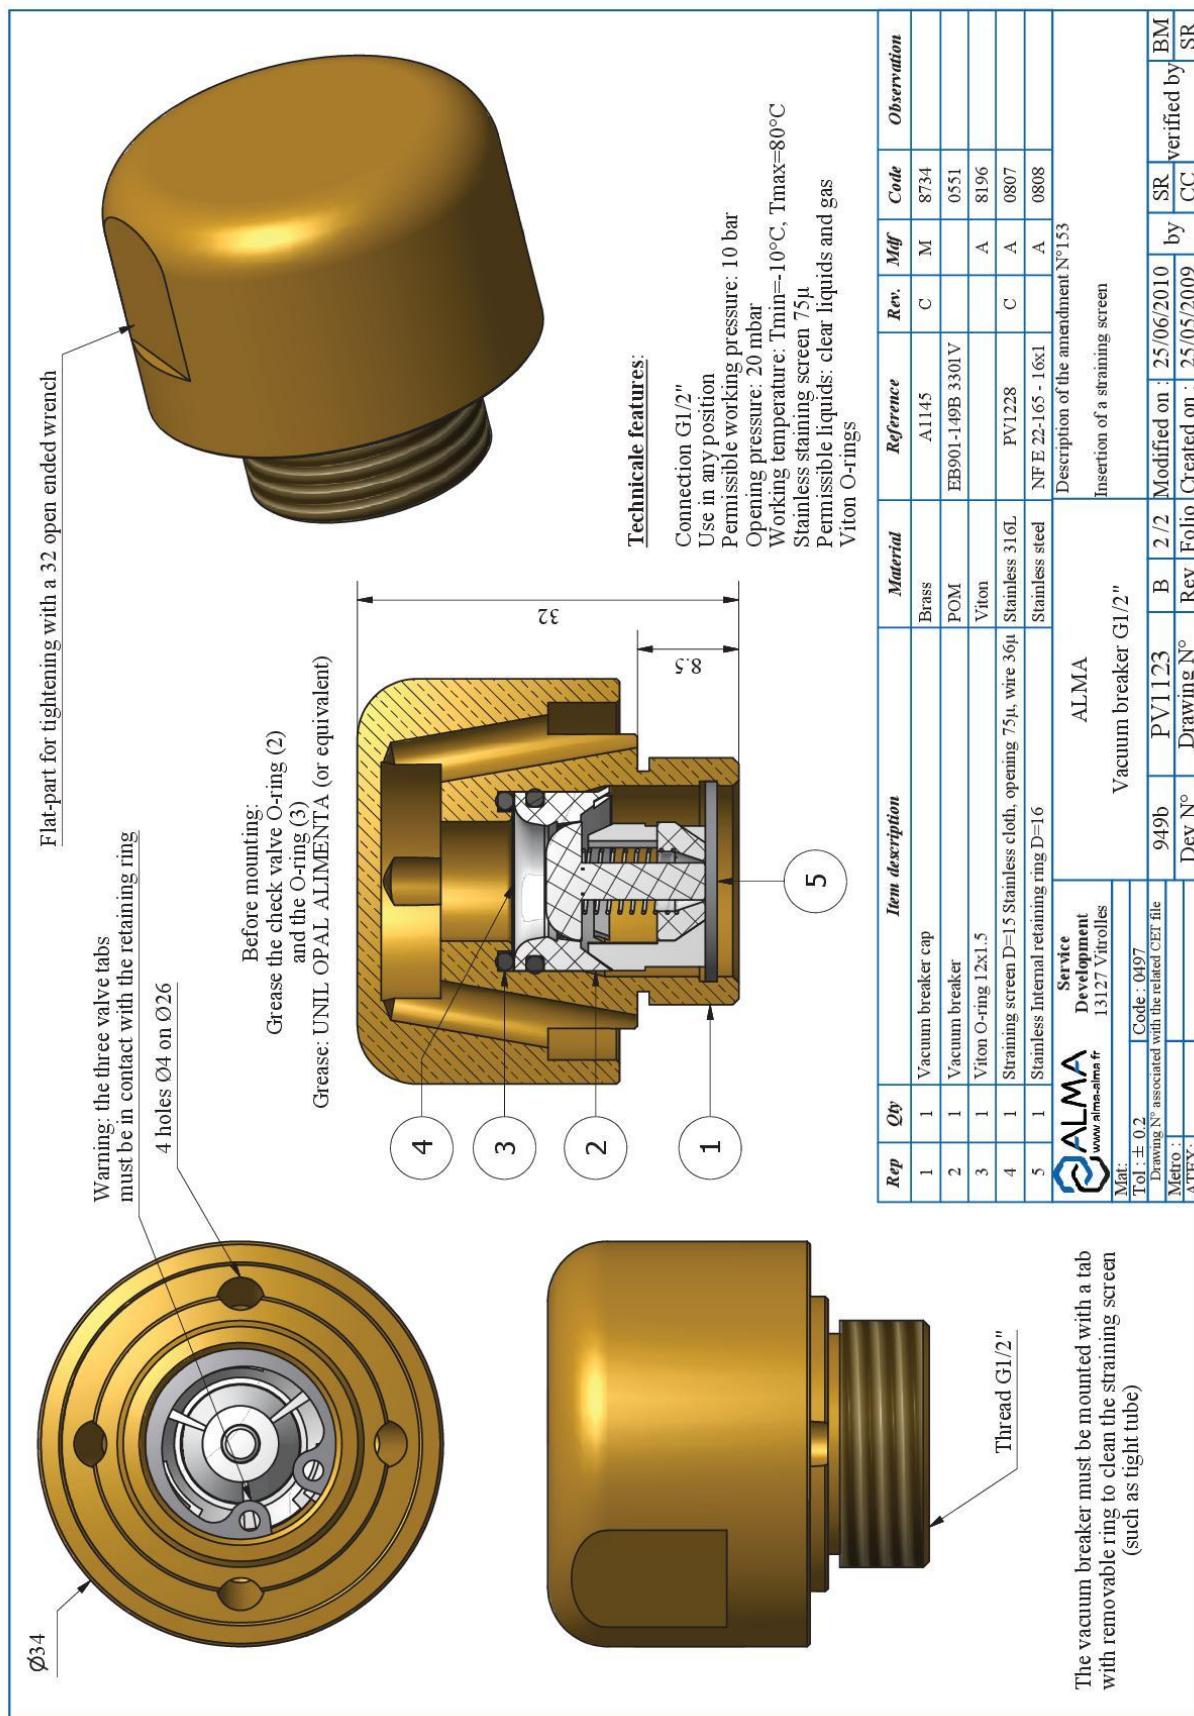


Document available on website [alma-alma.fr](http://www.alma-alma.fr)

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION	
	INSTALLATION GUIDE DI 015 ENE GRAVITRONIQUE This document is available at www.alma-alma.fr
	Units of measure: Length: mm Angle: degree (° °) Temperature: °C Page 36 / 47

12.1. INSTALLATION RECOMMENDATIONS VACUUM BREAKER

When associated to a measuring device, the vacuum breaker must be installed downstream.

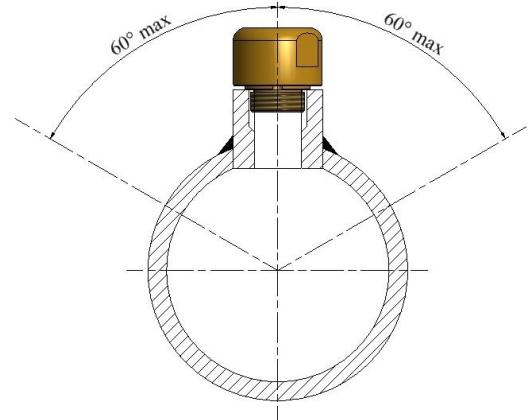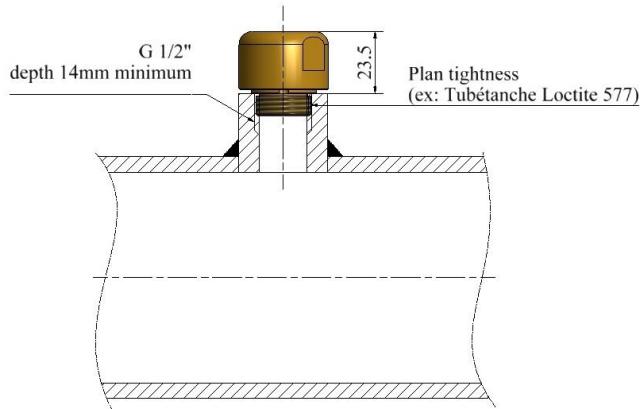

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY

THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION



INSTALLATION GUIDE DI 015 EN E
GRAVITRONIQUE

This document is available at www.alma-alma.fr


Units of measure:
Length: mm
Angle: degree (° ° °)
Temperature: °C

Page 37 / 47

13. DN80 NON-RETURN VALVE KITS**13.1. DN80 NON RETURN VALVE KIT, 0.03 BAR CALIBRATED**

DIMENSIONS FOR DN80 NON-RETURN VALVE KIT – 0.03 bar calibrated:

Ø144

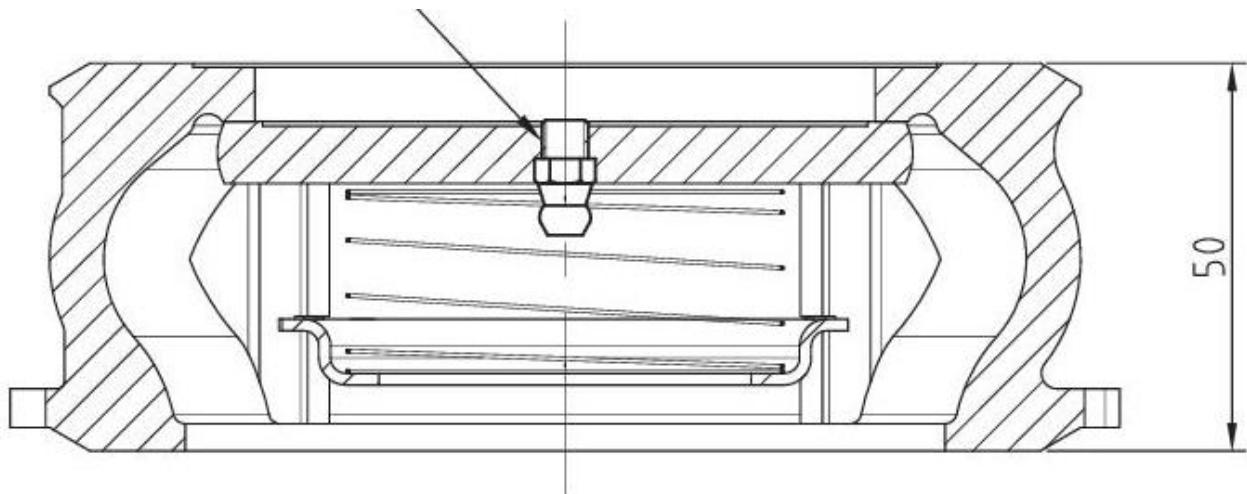

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY

THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION




INSTALLATION GUIDE DI 015 EN E
GRAVITRONIQUE

Units of measure:
Length: mm
Angle: degree (° ° °)
Temperature: °C

This document is available at www.alma-alma.fr

Page 38 / 47

13.2. DN80 NON RETURN VALVE KIT, 0.3 BAR CALIBRATED (EMPTY HOSE OPTION)

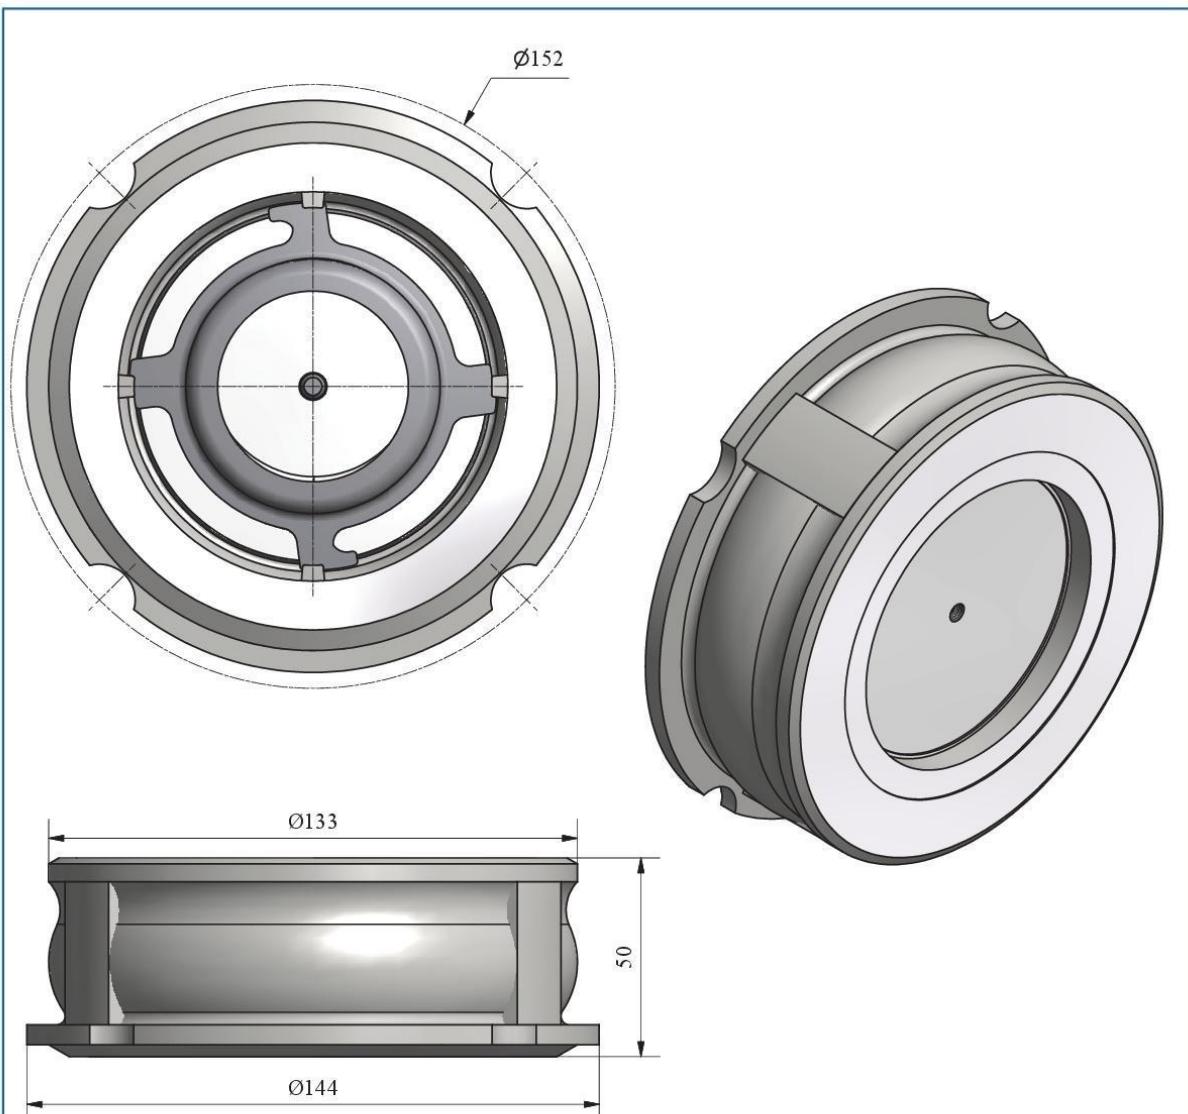


- Mass : ~ 2.5Kg
- Material : Inox 316L
- Operating temperature : -10°C to +350°C
- Permissible operating pressure : 40 bar
- Maximum permissible pressure :
 - Liquid 1: 25 bar
 - Gas 1: 12 bar
 - Liquid 2: 40 bar
 - Gas 2: 40 bar
- Pressure drop : 0.2 bar at 50 m3/h
- Mounting : Between downstream flange of the turbine
- Tightness : Flat gasket
- Standards :
 - CE conformity directive 97/23/CE
 - CE ATEX conformity directive 94/9/CE

 www.alma-alma.fr	Service Development		Kit non return valve, calibrated at 0.3 bar		Description of amendment N°				
	13127 Vitrolles		Adriane DN80 24X						
Mat:	Tol : ± 0.2	Code : 8798	905a	PV1908	A	2 / 2	Modified on :		by
Metro :		Drawing N° associated with the related CET file	Dev N°	Drawing N°	Rev	Folio	Created on :	29/03/2016	CC verified by SR
ATEX:									

	ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY							
	THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION							
	INSTALLATION GUIDE DI 015 ENE GRAVITRONIQUE							
This document is available at www.alma-alma.fr								Page 39 / 47

13.3. INSTALLATION RECOMMENDATIONS DN80 NON-RETURN VALVE KIT

- Refer to the certificate written on the identification plate of the measuring system to suit the sealing requirements
- No loose lead wire on the sealing devices

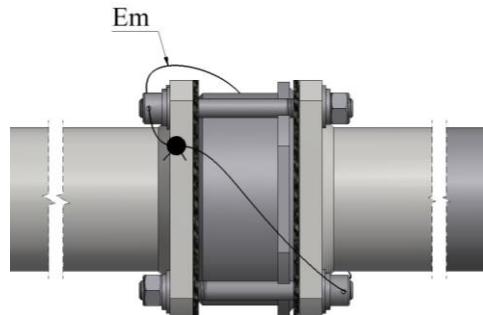


ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY

THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION

**INSTALLATION GUIDE DI 015 EN E
GRAVITRONIQUE****Units of measure:**
Length: mm
Angle: degree (° ° °)
Temperature: °CThis document is available at www.alma-alma.fr

Page 40 / 47

14. PNEUMATIC CONTROL VENT VALVE

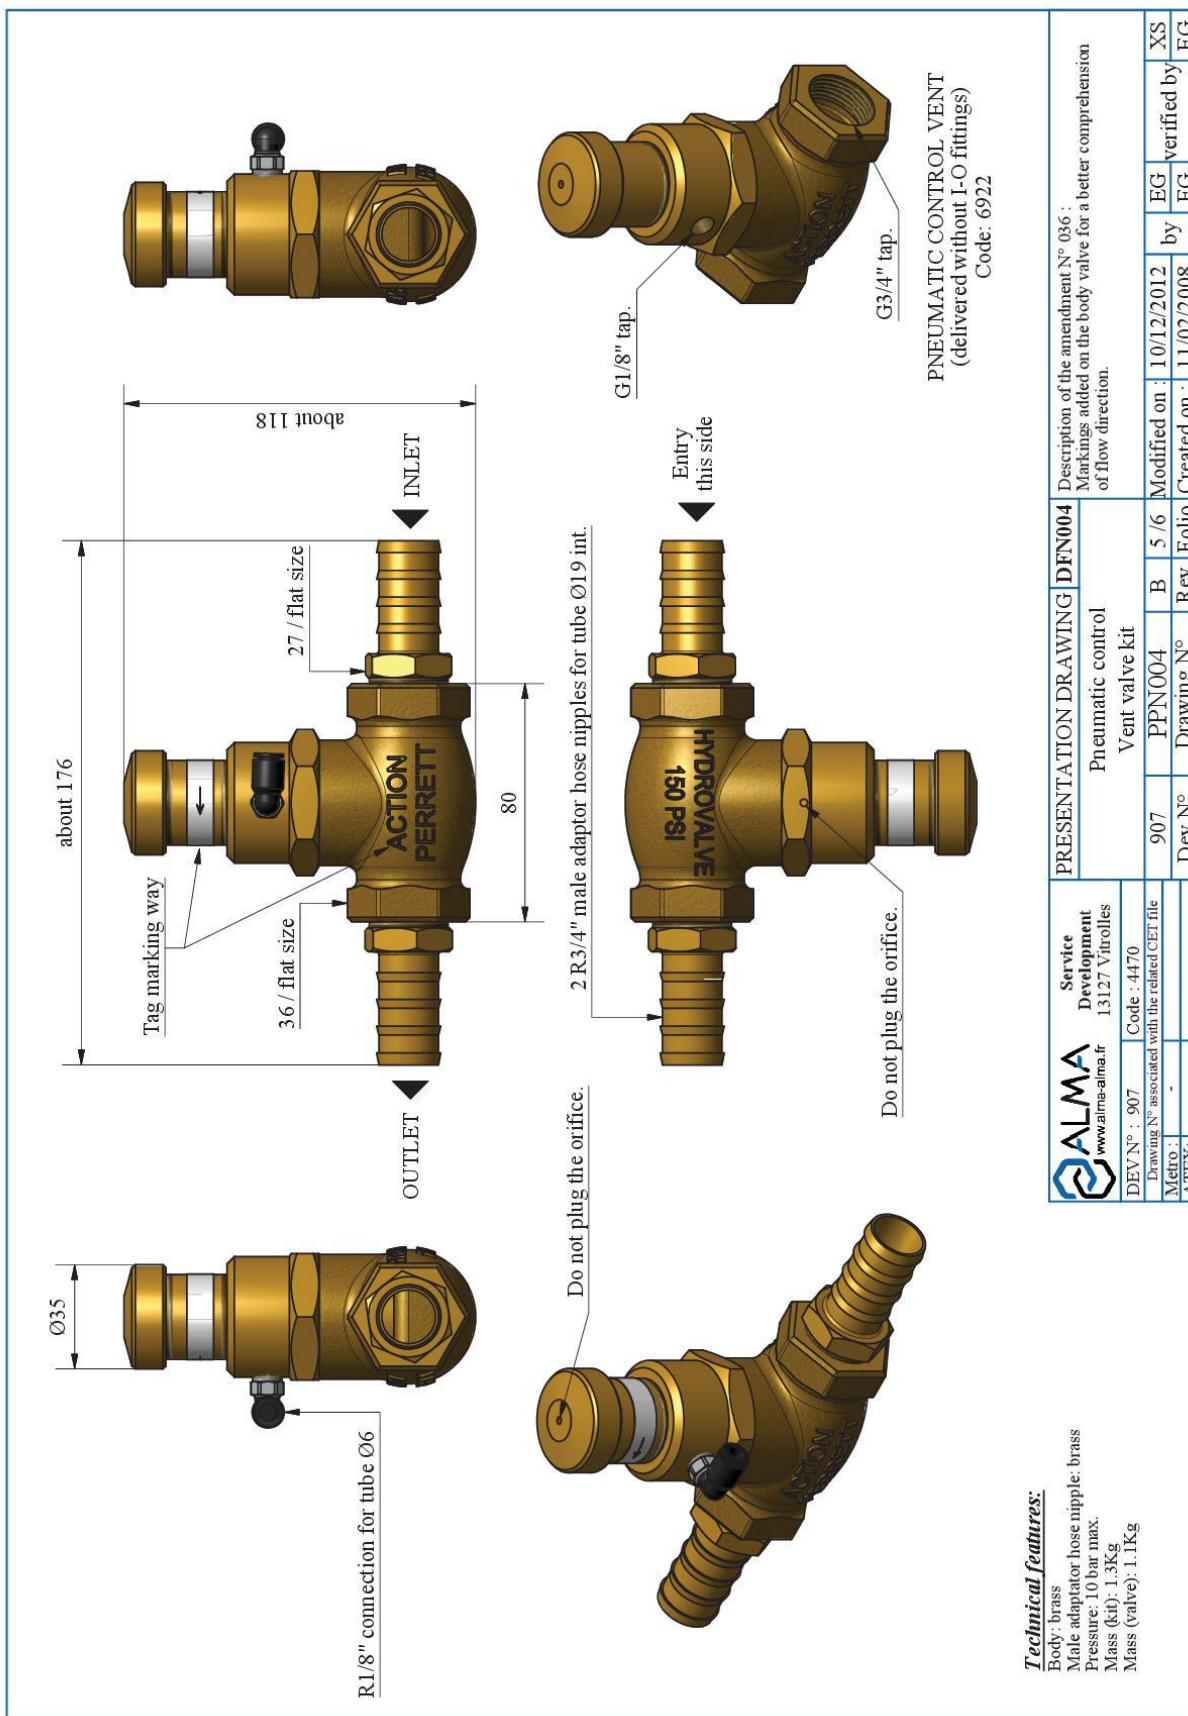


Technical features:

Body: brass
Male adaptor hose nipple: brass
Pressure: 10 bar max.
Mass (kit): 1.3Kg
Mass (valve): 1.1Kg


Description of the amendment N° 036 :
Markings added on the body valve for a better comprehension
of flow direction.

</

14.1. INSTALLATION RECOMMENDATIONS PNEUMATIC CONTROL VENT VALVE

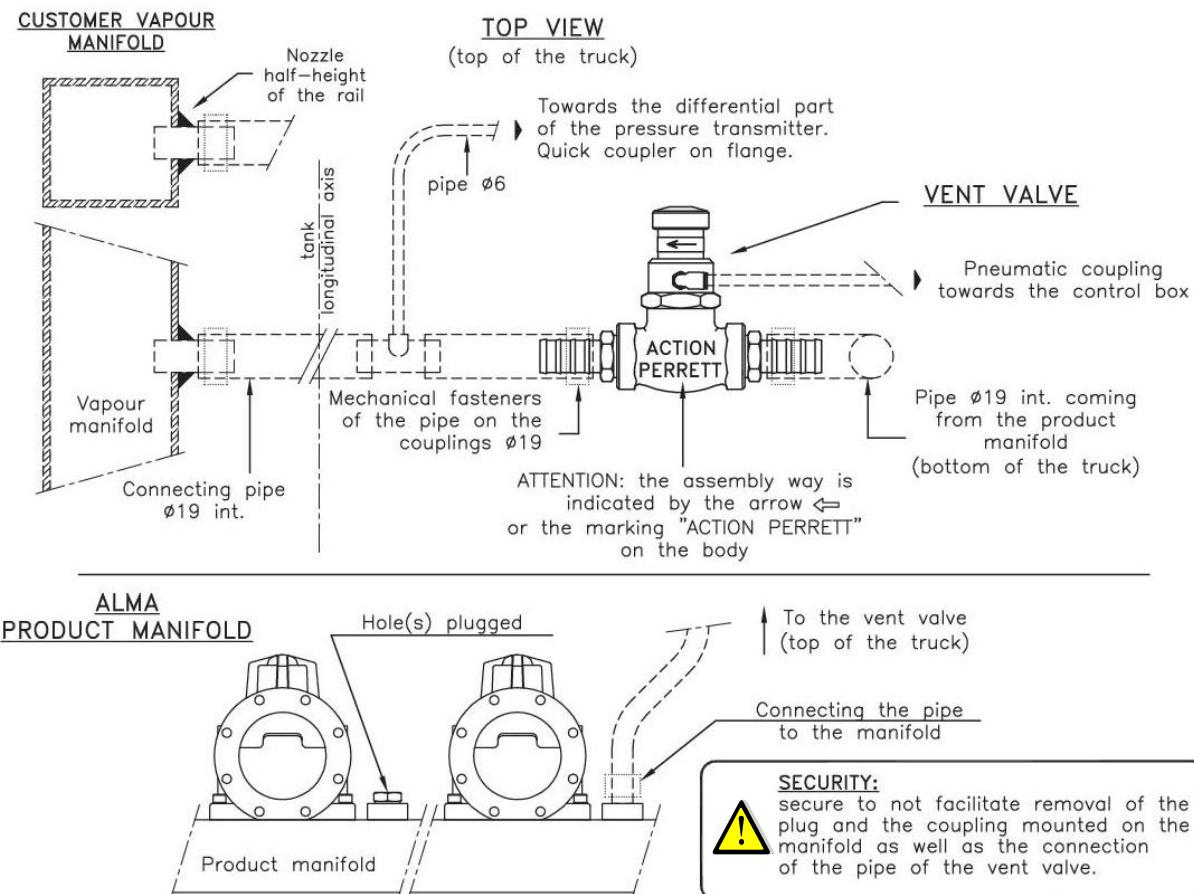

ASSEMBLY OF THE VENT PIPE (not supplied by Alma)

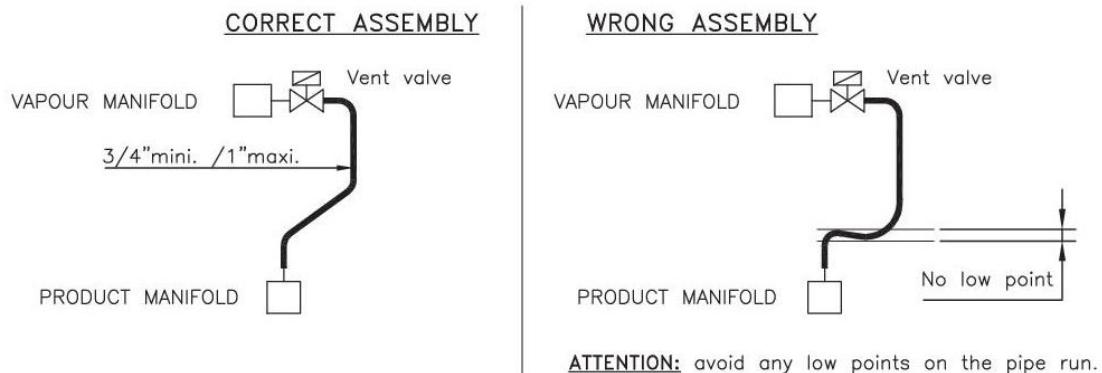

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY

THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION




INSTALLATION GUIDE DI 015 ENE
GRAVITRONIQUE

Units of measure:
Length: mm
Angle: degree (° ° °)
Temperature: °C

This document is available at www.alma-alma.fr

Page 42 / 47

15. TEMPERATURE PROBE Pt100 – CT1001

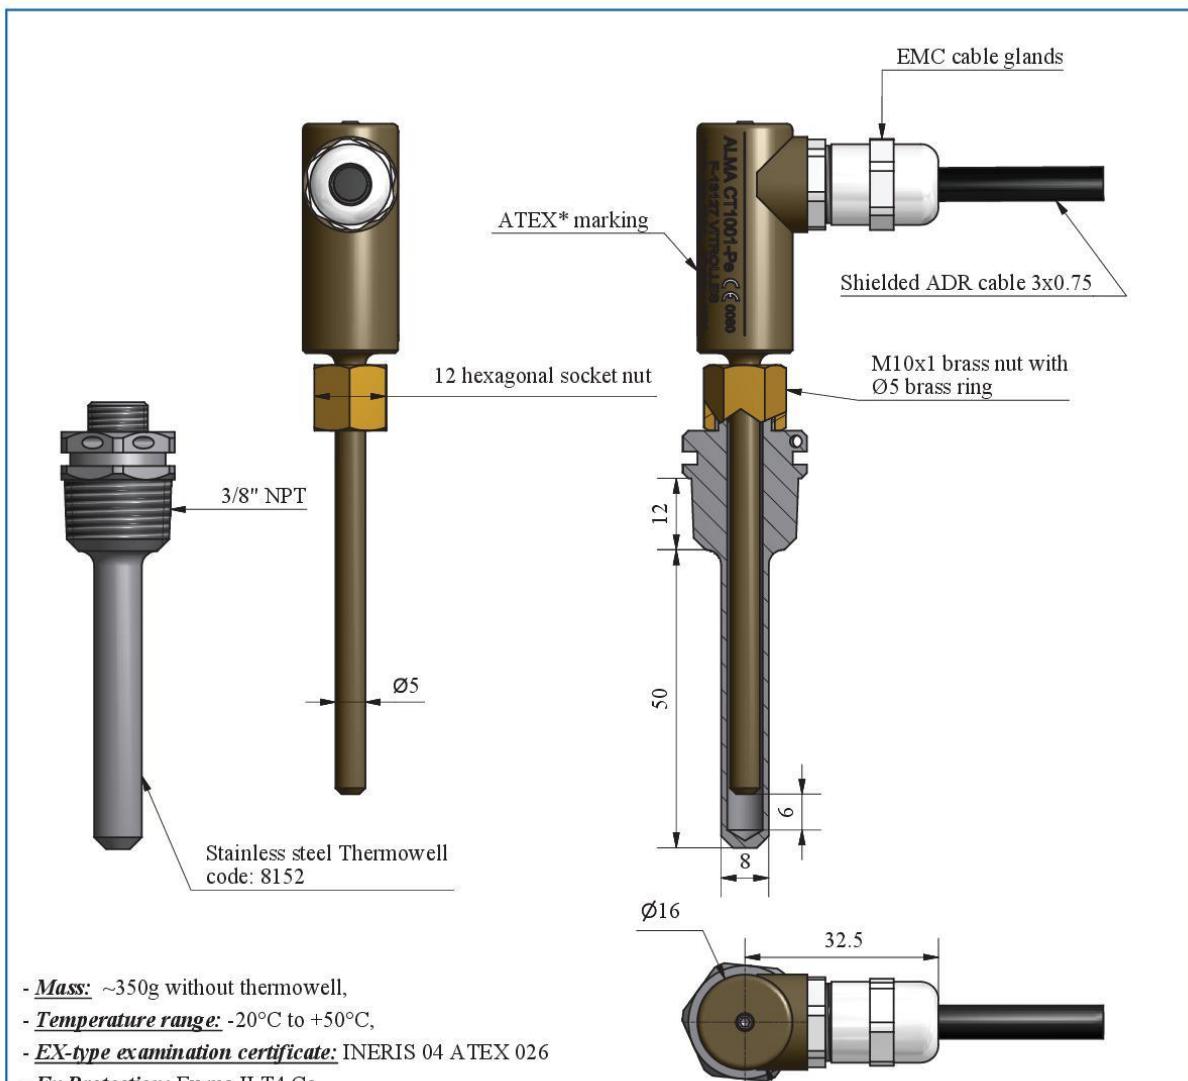

- **Mass:** ~350g without thermowell,
- **Temperature range:** -20°C to +50°C,
- **EX-type examination certificate:** INERIS 04 ATEX 026
- **Ex Protection:** Ex ma II T4 Ga

The sensor body is made of bronze color anodized aluminum alloy;
The ring and the nut are made of brass.
The probe can be mounted either on a ALMA thermowell or on a
thimble connection 1/4 "BSP (M10x1 n5).
Before installation, lubricate the parts in contact with the thermowell or
the boss, to prevent corrosion

PT100 features:

- 3 wires
- 1/3 DIN

*ATEX "ma" certification.

For installation and use in hazardous areas see Instruction manual


Also available with output connector according to IEC 60947-5-2

Connecting the cable		
Function	Marking on the wire	Color wire
PT100/1	1	Yellow
PT100/2	2	White
PT100/3	3	Green

ALMA www.alma-alma.fr Service Development 13127 Vitrolles DEV N° : 949d Code : 8151 Drawing N° associated with the related CET file Metro : ATEX :	PRESENTATION DRAWING DFV042				Description of the amendment N° 596			
	Temperature probe CT1001-Pe				- Compliance with ATEX marking - Replacement of the ADR cable - Modification of CI051			
949d	PPV042	K	5 / 7	Modified on : 21/02/2018	by ROC	verified by CC		
Dev N°	Drawing N°	Rev	Folio	Created on : 13/09/2003	by BM	verified by BM		

ALMA	ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY					
	THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION					
	INSTALLATION GUIDE DI 015 EN E GRAVITRONIQUE					
	This document is available at www.alma-alma.fr					Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C
						Page 43 / 47

15.1. INSTALLATION RECOMMENDATIONS TEMPERATURE PROBE

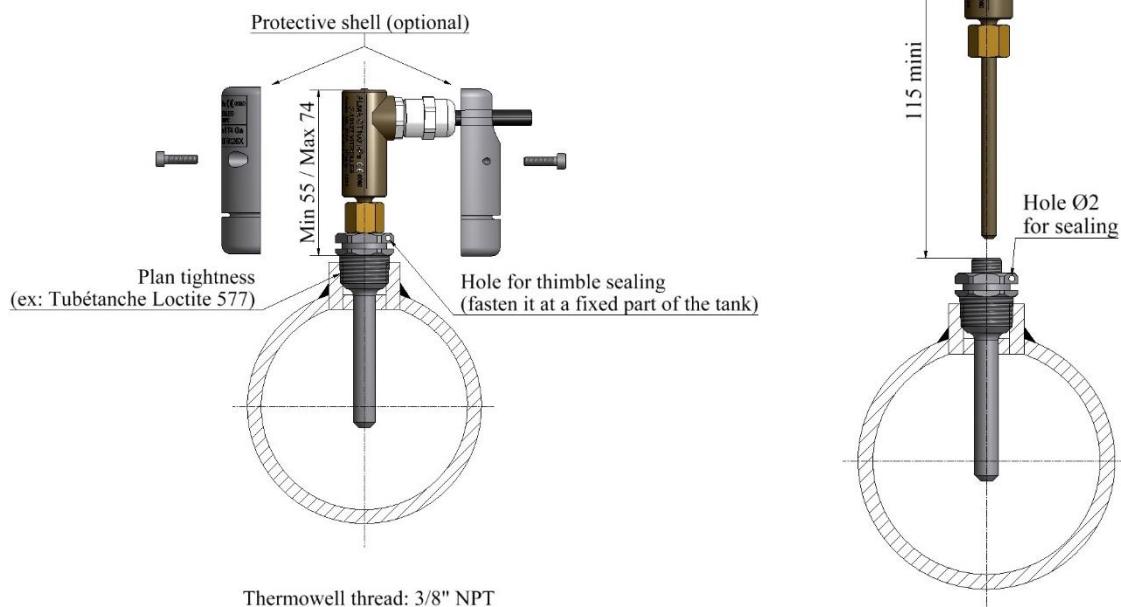

REFER TO INSTRUCTION MANUAL
(DELIVERED WITH THE EQUIPMENT AND AVAILABLE ON ALMA WEBSITE)

INSTALLATION OF THE TEMPERATURE SENSOR ON THE ALMA TURBINE METER:



ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY

THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION




INSTALLATION GUIDE DI 015 EN E GRAVITRONIQUE

This document is available at www.alma-alma.fr

Units of measure:
Length: mm
Angle: degree (° ° °)
Temperature: °C

Page 44 / 47

16. SIGHTGLASS KIT 110x110 ADRIANE TURBINE METER DN80

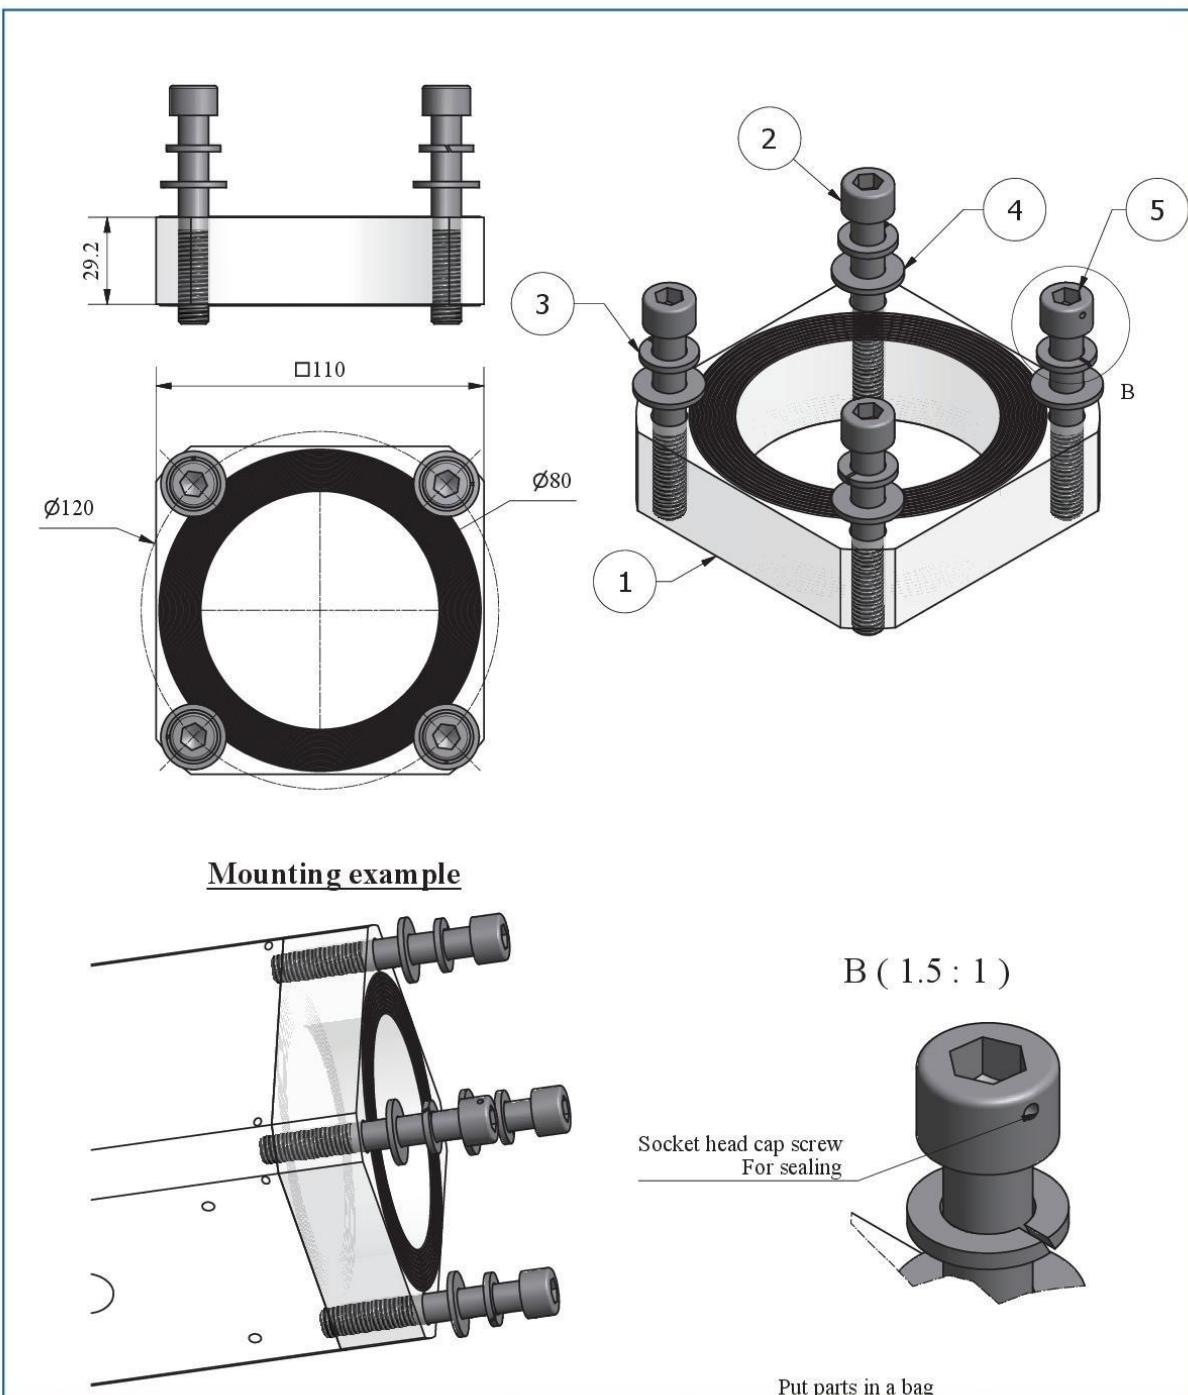

Rep	Qty	Item description	Material	Reference	Rev.	Mdf	Code	Observation
1	1	Sightglass DN80 110X110	Moulded PMMA	A0533	B		0908	
2	3	CHC screw M10 x 70 (ISO 4762)	Stainless A4-70				8595	
3	1	Washer W M10 (DIN 127)	Stainless A4-70				8474	
4	1	Washer M M10 (NFE 25-514)	Stainless A4-70				8430	
5	1	CHC screw M10 x 70 (ISO 4762) with head pierced	Stainless A4-70	PN0030	B	A	3465	

ALMA
www.alma-alma.fr
Service Development 13127 Vitrolles

Mat: Tol : ± 0.2 Drawing N° associated with the related CET file Dev N°

Adriane turbine meter DN80 24X

Description of amendment N°530
Integration of drill head screws

Metro : Rev Folio Created on : 30/03/2016 by CC verified by SR

ATEX: Drawing N°

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY								
THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION								
ALMA	INSTALLATION GUIDE DI 015 ENE GRAVITRONIQUE							Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C
	This document is available at www.alma-alma.fr							Page 45 / 47

16.1. INSTALLATION RECOMMENDATIONS SIGHTGLASS KIT DN80

- Refer to the certificate written on the identification plate of the measuring system to suit the sealing requirements
- No loose lead wire on the sealing devices




ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY

THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION

	INSTALLATION GUIDE DI 015 ENE GRAVITRONIQUE	Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C
	This document is available at www.alma-alma.fr	Page 46 / 47

17. KIT FOR MEASURING SYSTEM IDENTIFICATION PLATE

The identification plate shall be clearly installed, near the associated indicator device, and of easy access in order to be able to read features and to stamp the regulatory marks.

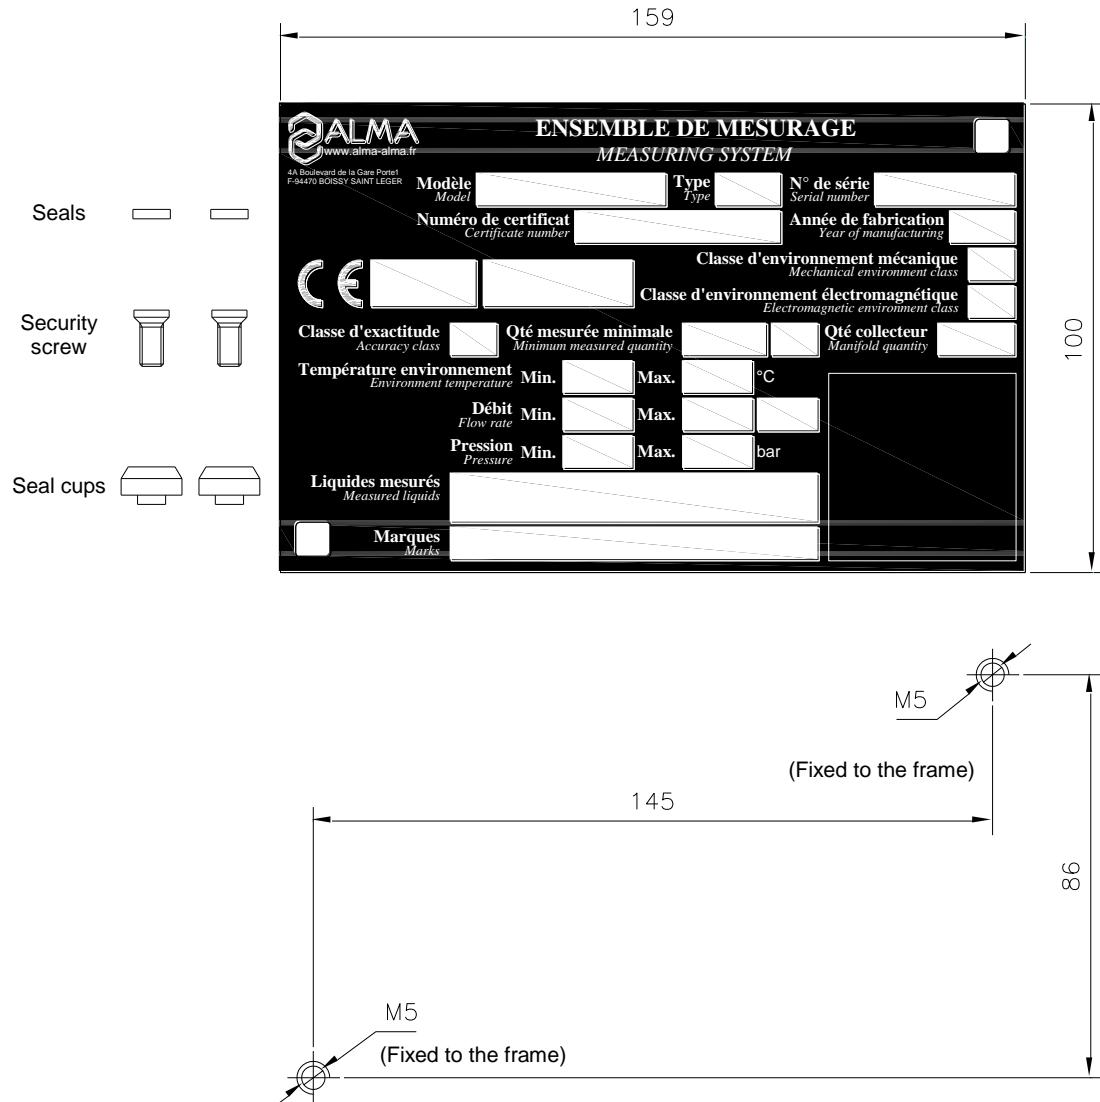

The security screws of the cups (provided by ALMA) must be screwed in the tap of the frame (do not use removable nuts).

ALL RECOMMENDATIONS ARE FOR REFERENCE ONLY		
THIS DOCUMENT IS THE PROPERTY OF ALMA. IT CAN BE NEITHER COPIED NOR COMMUNICATED TO ANY THIRD PARTIES WITHOUT ALMA AUTHORIZATION		
	INSTALLATION GUIDE DI 015 ENE GRAVITRONIQUE	Units of measure: Length: mm Angle: degree (° ° °) Temperature: °C
This document is available at www.alma-alma.fr		Page 47 / 47